


PULSE GENERATOR PERFORMANCE  
CHECK


Model: AVI-MP

S.N.: 118

Date: MAY 23 '77

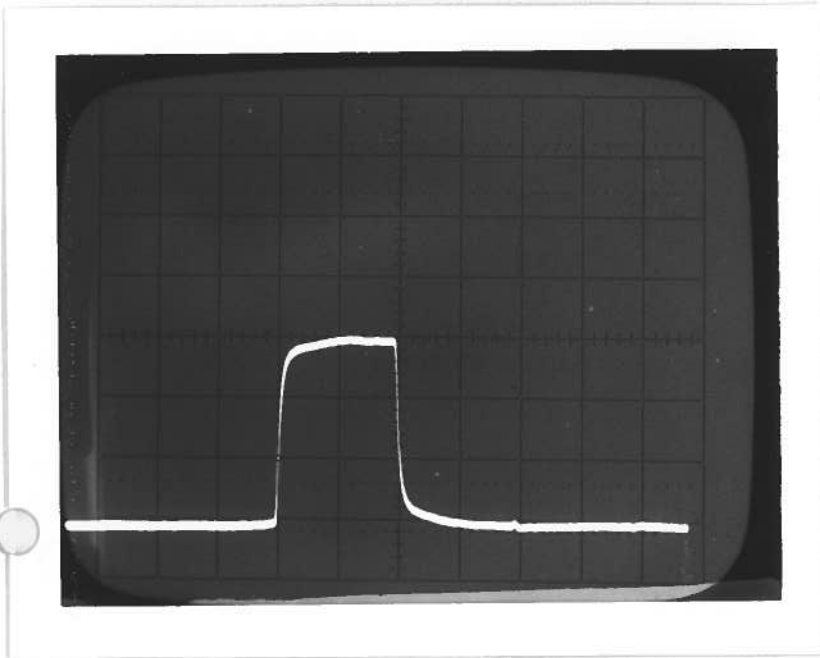

14 VOLTS/DIV, 10.0 NSEC/DIV  
(6.5 FOOT CABLE)

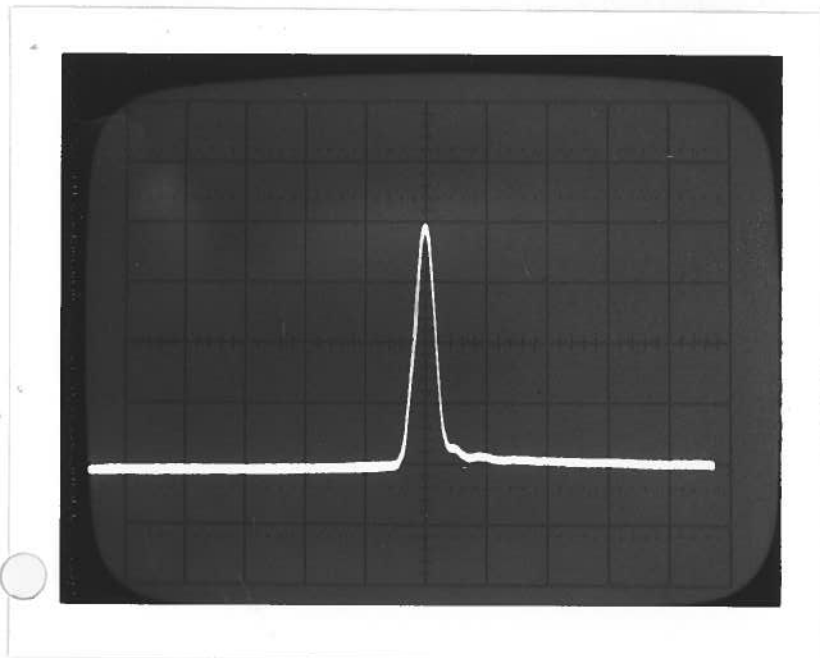

7 VOLTS/DIV, 1.0 NSEC/DIV  
NO EXTERNAL CABLE.

a) Output signal amplitude:

> 40 VOLTS.

b) Pulse width:

VARIABLE FROM 1.0 TO  
100 NSEC

c) Rise time:

≤ 0.5 NSEC

d) Fall time:

≤ 1.0 NSEC

e) PRF:

OK

f) Jitter, stability:

OK.

g) Prime power:

715 VOLTS @ < 120 m

A large, handwritten signature or scribble in black ink, located in the bottom right corner of the page.