


PULSE GENERATOR

PERFORMANCE CHECK

Model: *AVL-TN-1*
S.N.: *966*
Date: *1966 3082*

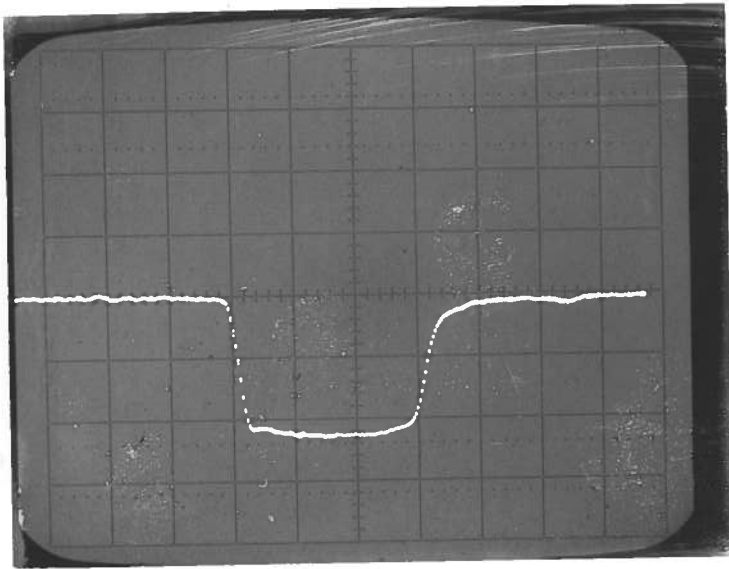

*100V/DIV.
10 nSEC/DIV.
2 kHz.*


- a) Output signal amplitude:
-230V
- b) Pulse width:
5 TO 100 nSEC
- c) Rise time:
≤ 2 nSEC
- d) Fall time:
≤ 3 nSEC
- e) PRF:
0 TO 5 kHz.
- f) Jitter, stability:
OK
- g) Prime power:
*120/240V,
50-60 Hz.*
- h) DC OFFSET:
*+30V,
6 mA (MAX).*
- i) PROP DELAY:
≤ 100 nSEC.

PULSE GENERATOR
PERFORMANCE CHECK

Model: 19L-7N-1

S.N.: 966 (REPAIRED JAN 87)

Date: JAN 9 87

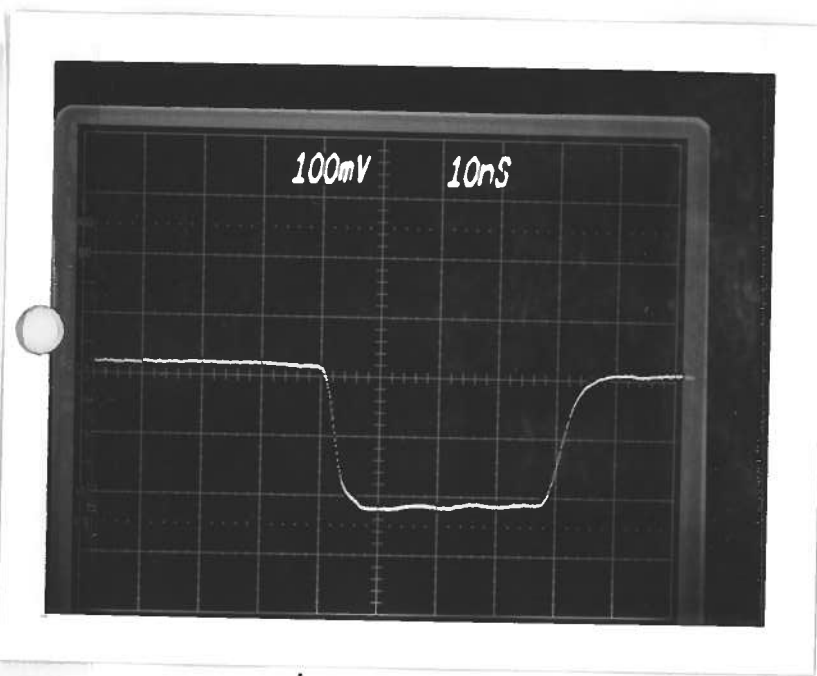

- a) Output signal amplitude:
-230 VOLTS, 0 OR
+30 VOLT OFFSET.
- b) Pulse width:
5 TO 100 NSEC.
- c) Rise time:
≤ 2 NSEC
- d) Fall time:
≤ 3 NSEC
- e) PRF:
0 TO 5 KHZ
- f) Jitter, stability:
OK
- g) Prime power:

60 dB ATTEN
100 VOLTS/DIV
2.0 KHZ

120/240 V
50-60 HZ