


PULSE GENERATOR  
PERFORMANCE CHECK

Model: *AVR-3-PW-CP-TR2*

S.N.: *7047*

Date: *MAY 30 1994*

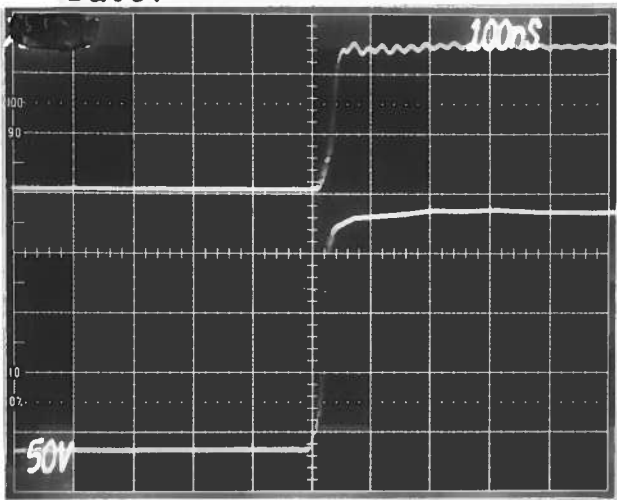


P6042 out

2 Amp/DIV

- a) Output signal amplitude:  
*0 TO +200 VOLTS TO 400 (5.0 AMP)*
- b) Pulse width:  
*0.25 TO 250 NS (0.25% MAX DUTY CYCLE)*
- c) Rise time:  
*≤ 20 NS*
- d) Fall time:  
*≤ 20 NS*
- e) PRF: *0 TO 10 KHZ (0.25% MAX DUTY CYCLE)*
- f) Jitter, stability:  
*OK*



(A) OVERSHOOT & RISE TIME CHECK

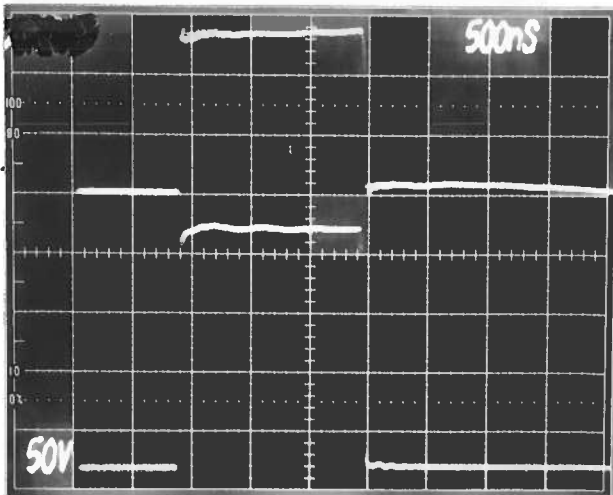

P6042 OUT  
2 Amp/DIV

- g) Prime power: *120/240V 50-60 HZ*

(B) NARROW PULSE PERFORMANCE (2 KHZ)

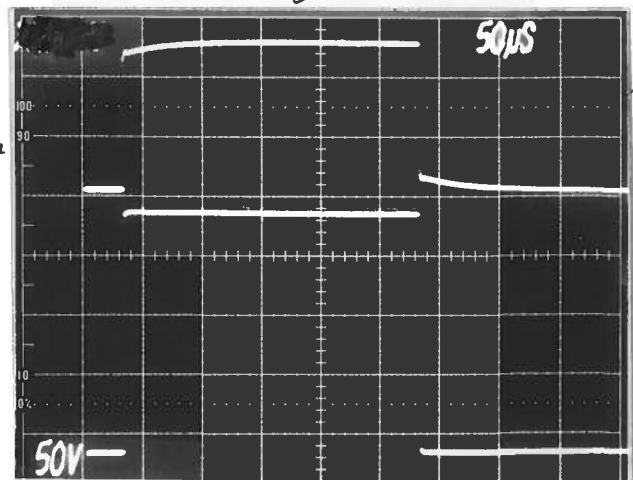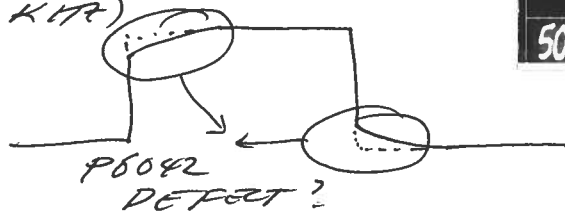

P604 OUT

P6106A OUT

WIDE PULSE PERFORMANCE (25 HZ)

*[Handwritten signature]*