


PULSE GENERATOR
PERFORMANCE CHECK

Model: AVP-2S-P-0S-ECL

S.N.: 7453

Date: SEPT 27 1995

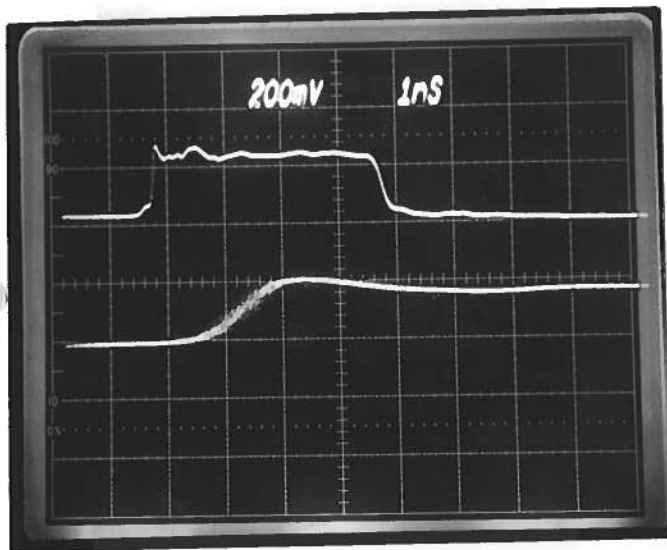

- a) Output signal amplitude:
0 TO +2 VOLTS -
- b) Pulse width:
0.2 TO 4.0 NS -
- c) Rise time:
1 NS/DIV ≤ 40 PS ✓
- d) Fall time:
50 PS/DIV ≤ 135 PS ✓
- e) PRF:
0 TO 1.0 MHz ✓
- f) Jitter, stability:
OK
- g) Prime power:
+15 VOLTS ✓
400 mA (MAX)

20 dB ATTEN
 $\therefore 2$ VOLTS/DIV
PRF = 1.0 MHz

$$T_{RT} = \sqrt{T_{R2S}^2 + T_{SCOPE}^2 + T_{ATTEN}^2}$$

≈ 50 PS (20-80%)

$$T_{SCOPE} = 25$$
 PS

18 GHz ATTEN + CABLES

\therefore CONC THAT $T_{R2S} \leq 40$ PS