


PULSE GENERATOR  
PERFORMANCE CHECK

Model: AVP-25-P-05-ECL

S.N.: 7454

Date: SEPT 27 1995

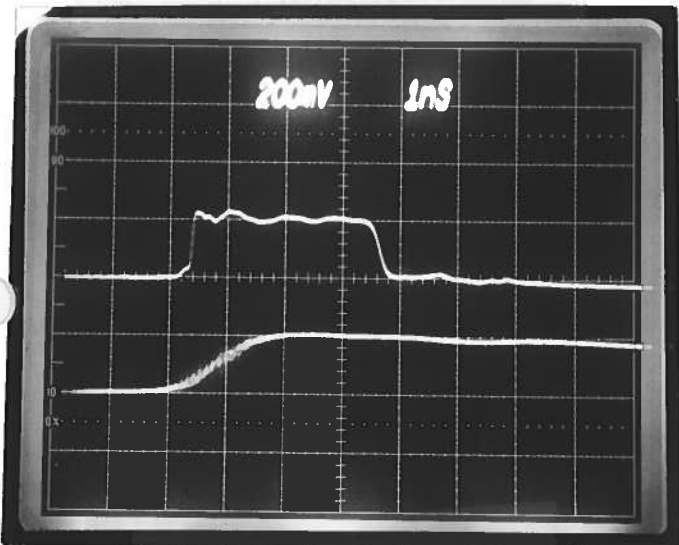

- a) Output signal amplitude:  
0 TO +2 VOLTS -
- b) Pulse width:  
0.2 TO 4.0 NS -
- c) Rise time:  
1 NS/DIV  
≤ 40 PS -
- d) Fall time:  
50 PS/DIV  
≤ 135 PS -
- e) PRF:  
0 TO 1.0 MHz -
- f) Jitter, stability:  
OK -
- g) Prime power:  
+15 VOLTS -  
400 mA (MAX) -

20 dB ATTEN  
∴ 2 VOLTS/DIV  
PRF = 1.0 MHz

$$T_{RT} = \sqrt{T_{R25}^2 + T_{SCOPE}^2 + T_{ATTEN}^2}$$

≈ 50 PS (20-80%)

$$T_{SCOPE} = 25 \text{ PS}$$

18 GHz ATTEN + CABLES

CONC THAT  $T_{R25} \leq 40 \text{ PS}$