

PULSE GENERATOR  
PERFORMANCE CHECK

Model: *AVO-6D-C-N-05-M*

S.N.: *9419*

Date: *Aug 23 2000*

- a) Output signal amplitude:  
*0 TO -10 AMP*
- b) Pulse width: *(0 TO -250 V TO 51 μs)*  
*50ns TO 5.0 μs*
- c) Rise time: *(0.5-1. MAX DUTY CYCLE)*  
*≤ 10 NS*
- d) Fall time:  
*≤ 10 NS*
- e) PRF: *0 TO 10 KHz*
- f) Jitter, stability: *(0.5% MAX DUTY CYCLE)*  
*OK*
- g) Prime power:  
*120/240 V*  
*50-60 Hz*




9419

AVO-6D-T OUTPUT.


TEK CT-2 CURRENT PROBE.

1 Amp/DIV OR 1 Amp/VOLT.

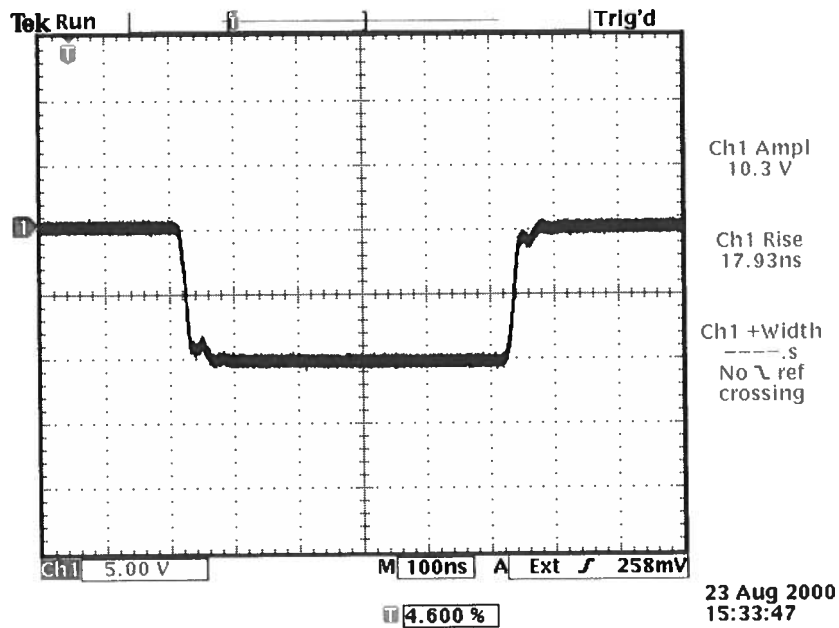

9419

MANFRAME OUT TO SDN  
NARROW PULSE

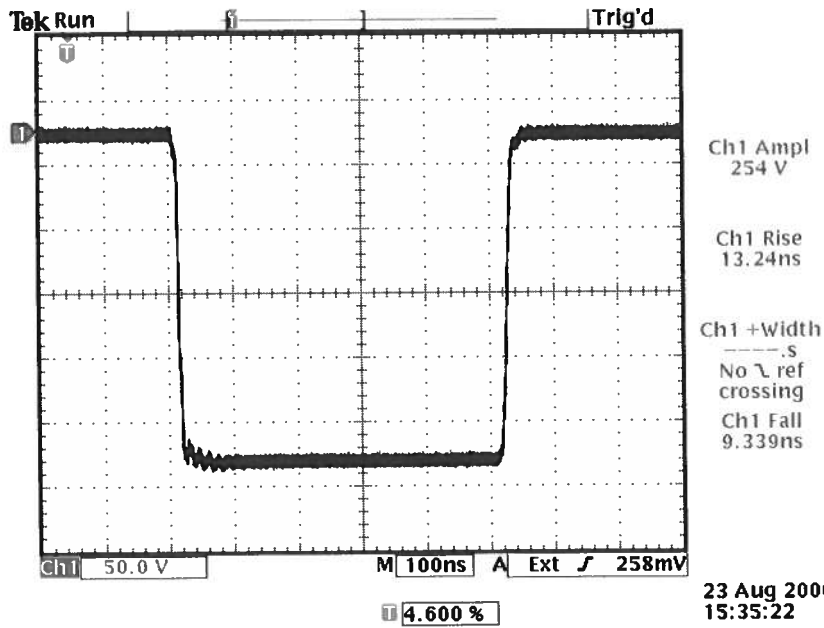

9419

MAINTAINING OUT TO 50Ω  
WIDE PULSE

