


PULSE GENERATOR

ACCEPTANCE TEST REPORT/PERFORMANCE CHECK SHEET

Model: AVO-2-C-BE03-R5-P-0PI-M

S.N.: 10143

Date: JAN 18 2002

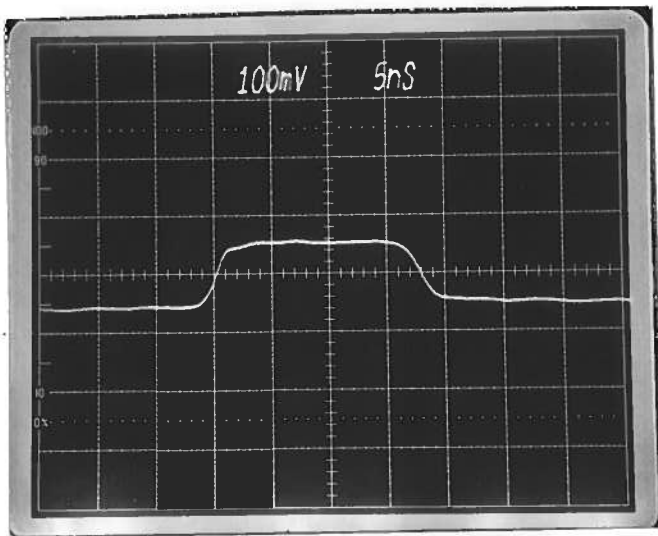

a) Output signal amplitude:

0 TO +2 AMP ✓

b) Pulse width:

17 NS ✓

c) Rise time: ✓

≤ 2 NS ✓

d) Fall time: ✓

≤ 2 NS

e) PRF:

0 TO 20 kHz ✓

f) Jitter, stability:

OK ✓

g) Prime power:

120/240V, 50-60 Hz ✓

MONITOR OUT TO 40 dB

100V/DIV, 2 AMP/DIV

5 NS/DIV

AVO-2T-BE02B3 CONNECTED

VIA A 8 METER CABLE

IN459A IN SERIES WITH

1 Ω USED AS TEST LOAD.

PRF = 20 kHz