



AVTECH ELECTROSYSTEMS LTD.
NANOSECOND WAVEFORM ELECTRONICS

P.O. BOX 265
OGDENSBURG, NY
U.S.A. 13669-0265
TEL: (315) 472-5270
FAX: (613) 226-2802

BOX 5120 STN. F
OTTAWA, ONTARIO
CANADA K2C 3H4
TEL: (613) 226-5772
FAX: (613) 226-2802

INSTRUCTIONS

MODEL AVO-7D-C-P-FP2 PULSE GENERATOR


S.N.:

WARRANTY

Avtech Electrosystems Ltd. warrants products of its manufacture to be free from defects in material and workmanship under conditions of normal use. If, within one year after delivery to the original owner, and after prepaid return by the original owner, this Avtech product is found to be defective, Avtech shall at its option repair or replace said defective item. This warranty does not apply to units which have been disassembled, modified or subjected to conditions exceeding the applicable specifications or ratings. This warranty is the extent of the obligation or liability assumed by Avtech with respect to this product and no other warranty or guarantee is either expressed or implied.

Fig. 1

PULSE GENERATOR TEST ARRANGEMENT

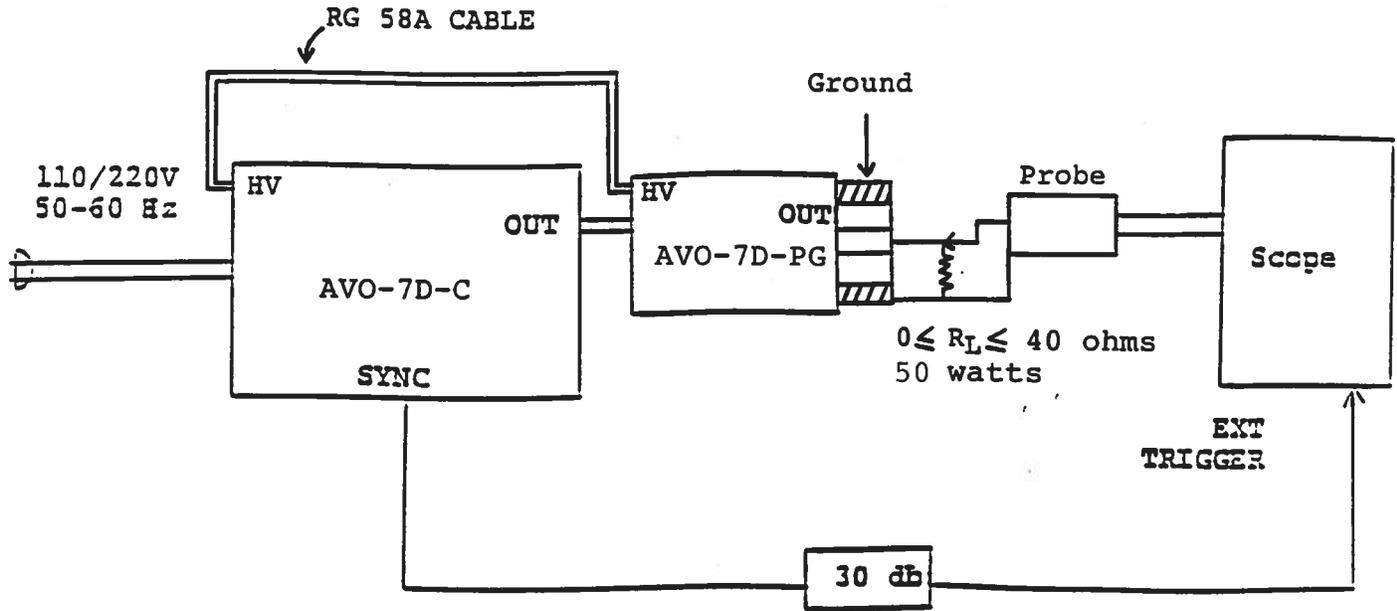

GENERAL OPERATING INSTRUCTIONS

- 1) The equipment should be connected in the general fashion shown above. Since the AVO unit provides an output pulse rise time as low as 100 ns a fast oscilloscope (at least 50 MHz and preferably 200 MHz) should be used to display the waveform. The mainframe and the -PG output module must be connected as shown in Fig. 1. Note that the HV port on the -PG module and the HV port on the rear panel of the mainframe must be connected by the RG-58A cable.
- 2) The TRIG output channel provides TTL level signals. To avoid overdriving the TRIG input channel of some scopes, a 30 db attenuator should be placed at the input to the scope trigger channel. The TRIG output precedes the main output when the front panel LEAD-LAG switch is in the LEAD position. The TRIG output lags the main output when the switch is in the LAG position.
- 3) To obtain a stable output display the PW and PRF controls on the front panel should be set mid-range. The front panel TRIG toggle switch should be in the INT position and the Mode A-B switch should be in the A position. The DELAY controls and the scope triggering controls are then adjusted to obtain a stable output. The scope may then be used to set the desired PRF by rotating the PRF controls. CAUTION: Do not exceed the duty cycle rating of 2.0% at maximum output current.
- 4) The output amplitude is controlled by the front panel ten turn Amp control.
- 5) An external clock may be used to control the output PRF of the unit by setting the front panel TRIG toggle switch in the EXT position and applying a 0.2 us (approx) TTL level pulse to the TRIG BNC connector input. For operation in this mode, the scope time base must also be triggered by the external clock rather than from the TRIG output.
- 6) When triggered externally, the output pulse width will equal the input trigger pulse width if the Mode A-B switch is in the B position. When the switch is in the A position, the output pulse width is controlled by the front panel controls.
- 7) The AVO-7D is designed to supply up to 40 ampere to a maximum load voltage of 40 volts. Factory tests are conducted with 1.2 ohm and 0.2 ohm loads capable of dissipating at least 50 watts. Higher load resistance values may be used but the output voltage must be limited to 40 volts or less.

- 8) The output terminals of the pulse generator module consists of a short length of microstrip transmission line protruding from the module chassis. The OUT terminal is the center conductor which is bounded on both sides by the ground plane (see below). Note that the "OUT" red banana terminal is in parallel with the microstrip center conductor and so may also be used as the output terminal. Note that the unit is designed to pulse resistive loads and will exhibit a large output spike when used to drive a load with significant inductance (LENZ'S LAW). For this reason the load should be connected to the output using low inductance leads (as short as possible and as heavy a gauge as possible).
- 9) Note that the HV BNC connector on the PG module must be connected to the rear panel HV BNC connector on the mainframe.
- 10) The unit can be converted from 110 to 220V 50-60 Hz operation by adjusting the voltage selector card in the rear panel fused voltage selector cable connector assembly.
- 11) If application assistance is required, call (613) 226-5772 or Fax (613) 226-2802.

AVO-7D-PG


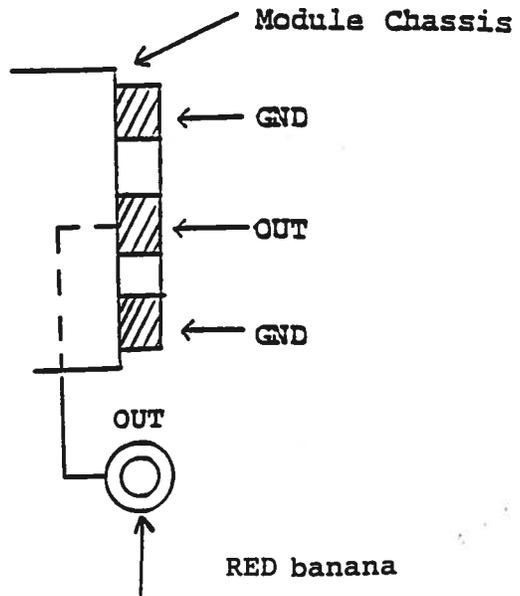


Fig. 2

FRONT PANEL CONTROLS

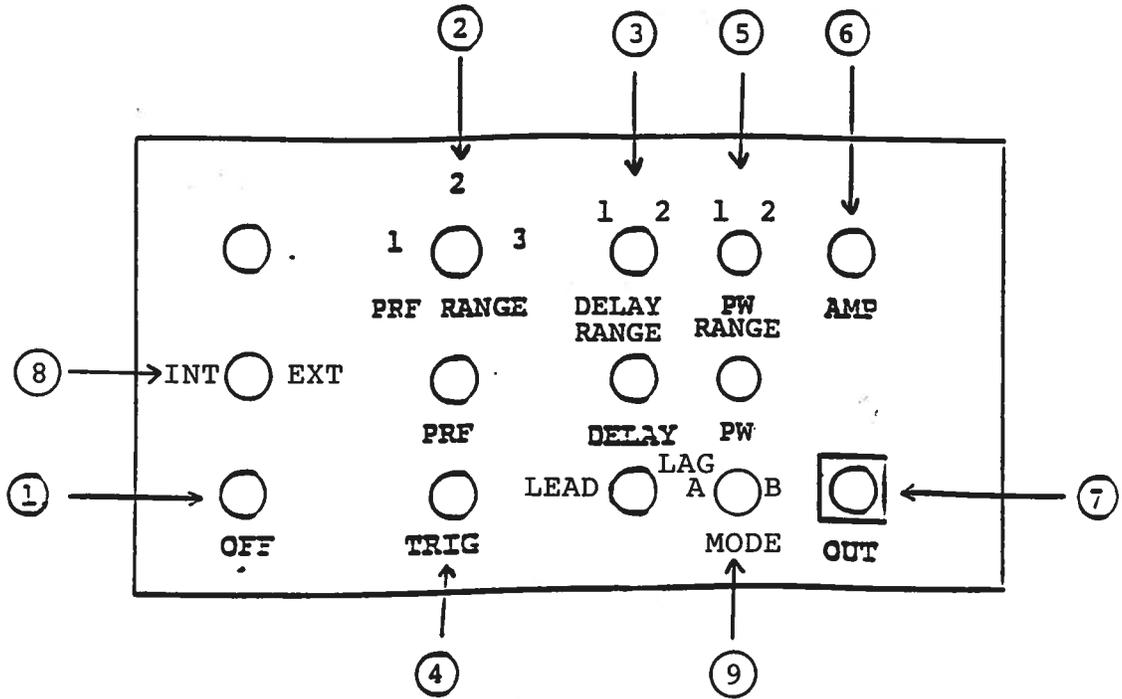

- (1) ON-OFF Switch. Applies basic prime power to all stages.
- (2) PRF Control. Varies PRF from 10 Hz to 10 kHz as follows:

Range 1	10 Hz to 100 Hz
Range 2	100 Hz to 1.0 kHz
Range 3	1.0 kHz to 10 kHz

- (3) DELAY Control. Controls the relative delay between the reference output pulse provided at the TRIG output (4) and the -PG output. This delay is variable as follows:

Range 1	0.2 us to 2 us
Range 2	2 us to 20 us

The TRIG output precedes the main output when the LEAD-LAG switch is in the LEAD position and lags when the switch is in the LAG position.


- (4) TRIG Output. This output is used to trigger the scope time base. The output is a TTL level 100 ns (approx.) pulse capable of driving a fifty ohm load.
- (5) PW Control. A one turn control and 2 position range switch which varies the output pulse width as follows (when the MODE A-B switch is in the A position):

Range 1	0.5 us to 5.0 us
Range 2	5.0 us to 50 us

- (6) AMP. A ten turn pot for controlling the output pulse amplitude.
- (7) OUT Connector. A multi pin connector which attaches the 2 foot cable from the pulse generator module to the main frame.
- (8) EXT-INT Control. With this toggle switch in the INT position, the PRF of the AVO unit is controlled via an internal clock which in turn is controlled by the PRF controls. With the toggle switch in the EXT position, the AVO unit requires a 0.2 us TTL level pulse applied at the TRIG input in order to trigger the output stages. In addition, in this mode, the scope time base must be triggered by the external trigger source.
- (9) MODE A-B. With this switch in the A position, the output pulse width is controlled by the front panel controls. When the switch is in the B position and the unit is triggered externally, the output pulse width equals the input trigger pulse width.

Fig. 3


BACK PANEL CONTROLS

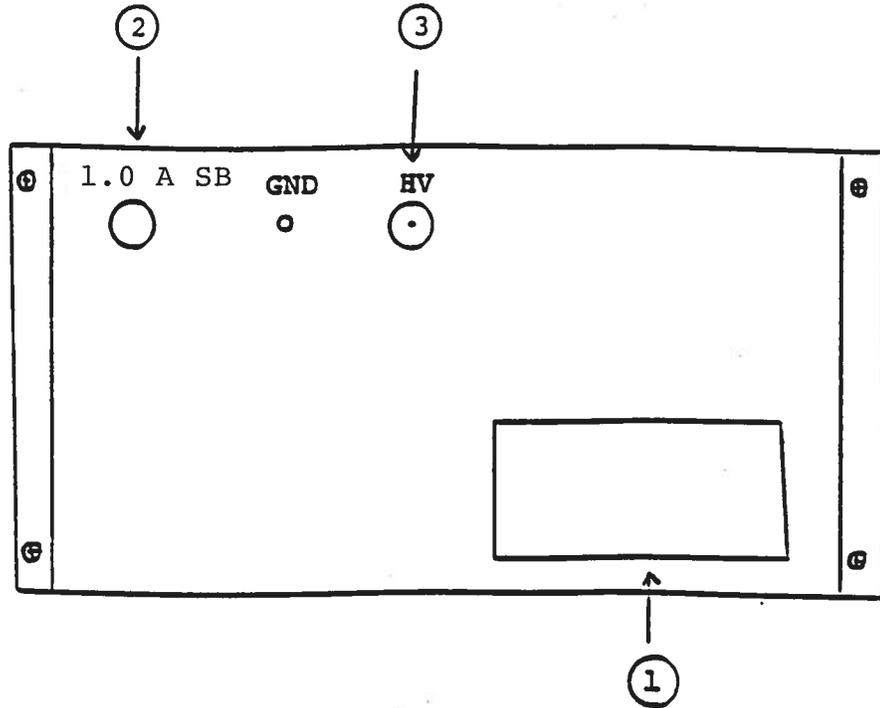

- (1) FUSED CONNECTOR, VOLTAGE SELECTOR. The detachable power cord is connected at this point. In addition, the removable cord is adjusted to select the desired input operating voltage. The unit also contains the main power fuse (1.0A SB).
- (2) 1.0 A SB FUSE. Protects output stage against overload conditions.
- (3) HV Connector. 100 foot long RG58 cable from -PG module HV BNC connects to this BNC connector. Supplies +65V volts from mainframe to -PG module.

Fig. 4

SYSTEM BLOCK DIAGRAM

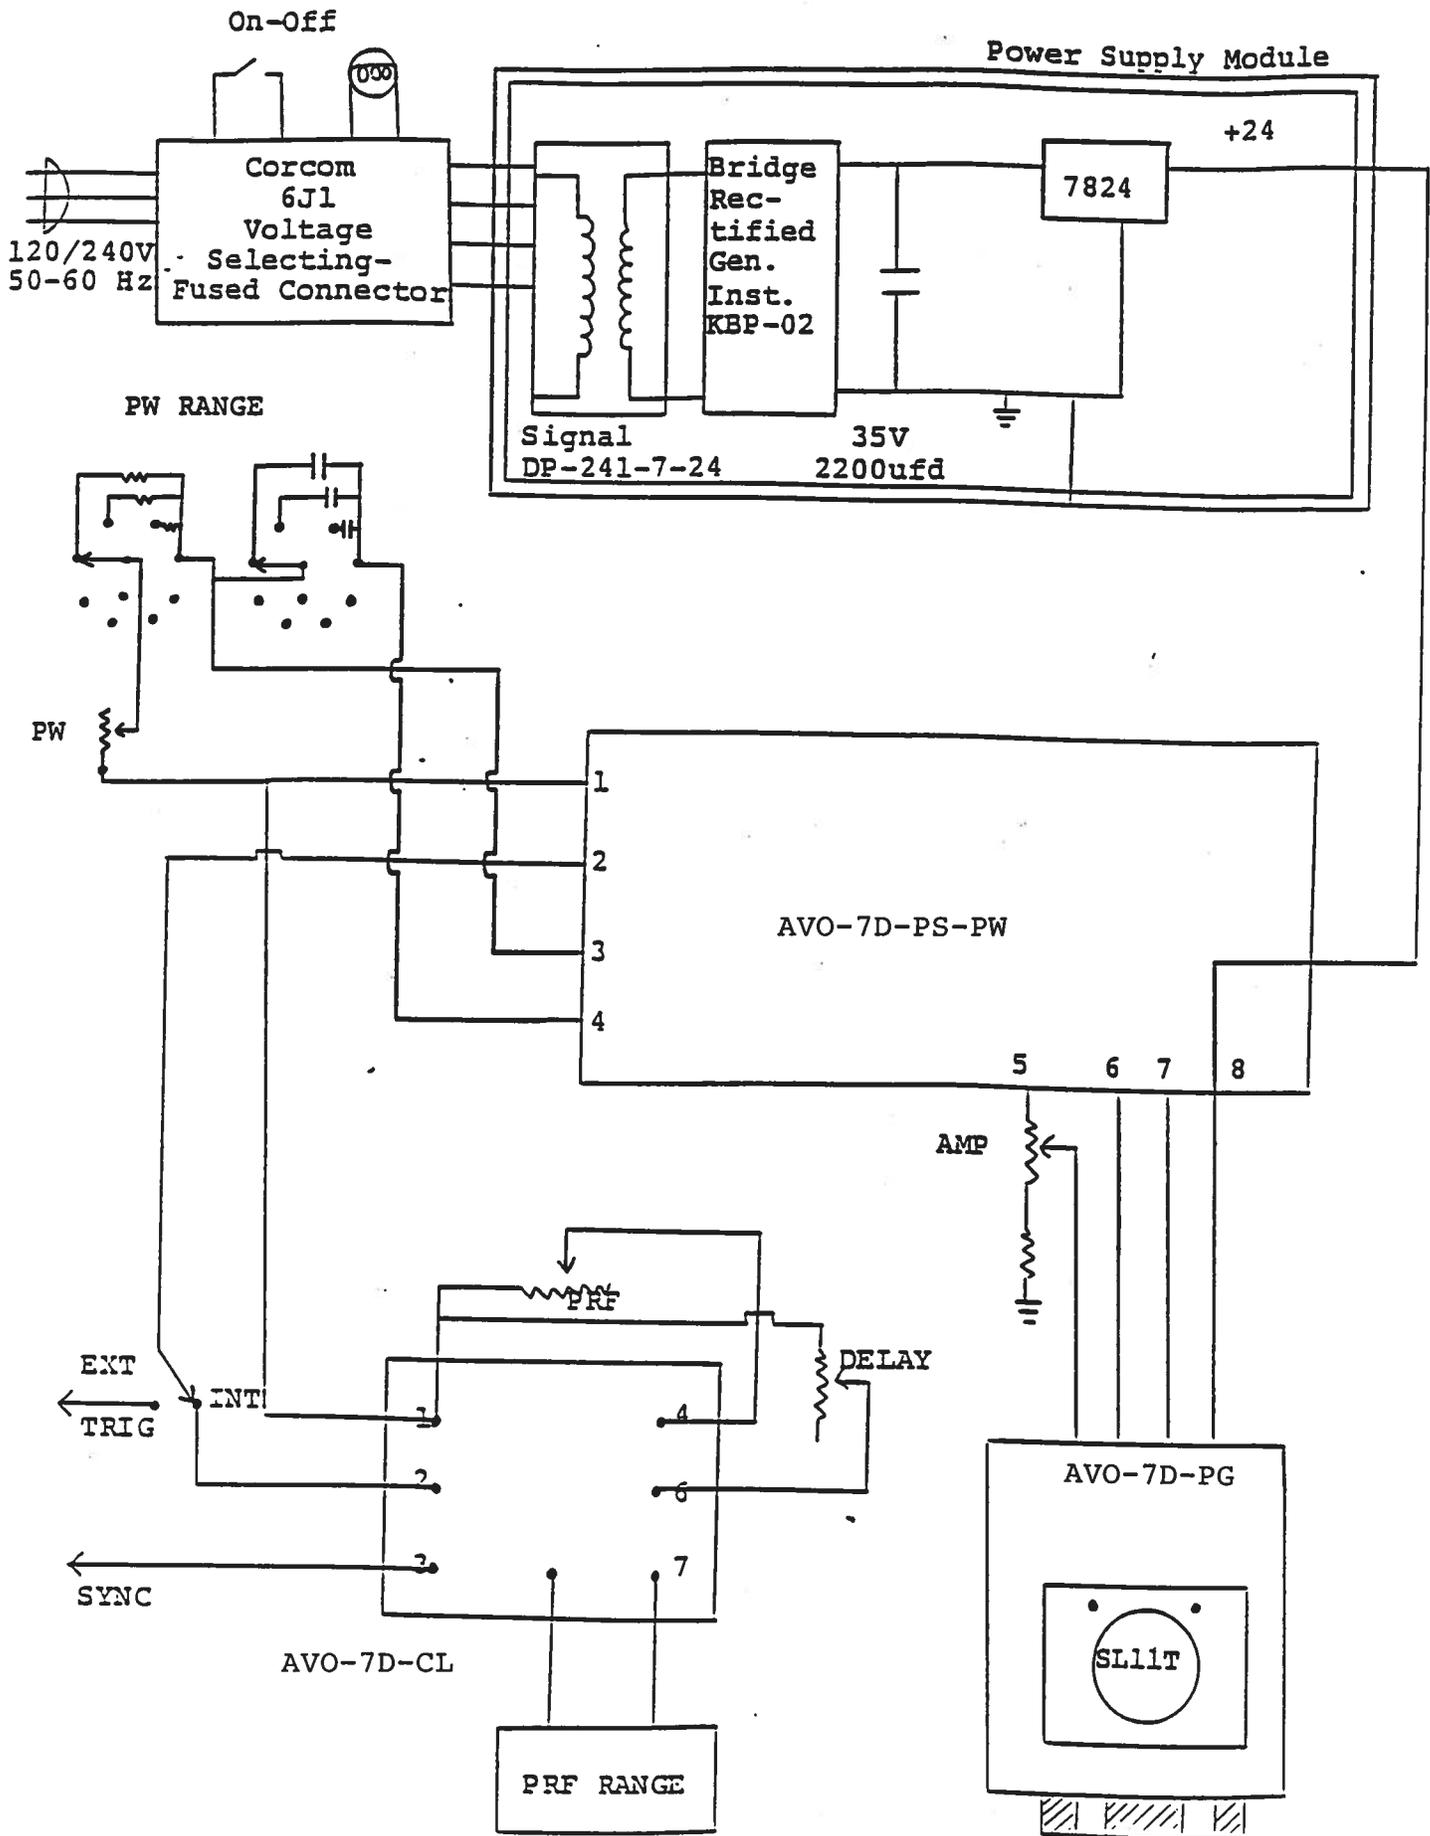

SYSTEM DESCRIPTION AND REPAIR PROCEDURE

The AVO-7D-C unit consists of the following basic modules:

- 1) AVO-7D-PG pulse generator module
- 2) AVO-7D-CL clock module
- 3) AVO-7D-PW pulse width control module
- 4) +24V power supply board and +65 volt power supply board

The modules are interconnected as shown in Fig. 4.

In the event of an instrument malfunction, it is most likely that the 1.0A slow blow fuse or the main line fuse (1.0 Amp) on the rear panel has blown. Replace if necessary. If the unit still does not function, it is most likely that some of the output switching elements may have failed and the unit should be returned to the factory for repair.

Schroff

05.06.92

Faint, illegible text, possibly bleed-through from the reverse side of the page.