



AVTECH ELECTROSYSTEMS LTD.

NANOSECOND WAVEFORM ELECTRONICS
SINCE 1975

P.O. BOX 265
OGDENSBURG, NY
U.S.A. 13669-0265

TEL: 888-670-8729 (USA & Canada) or +1-613-226-5772 (Intl)
FAX: 800-561-1970 (USA & Canada) or +1-613-226-2802 (Intl)

info@avtechpulse.com - <http://www.avtechpulse.com/>

BOX 5120, LCD MERIVALE
OTTAWA, ONTARIO
CANADA K2C 3H4

INSTRUCTIONS

MODEL AVR-G1-C-EMRA-P

0 TO +240 VOLTS, 10 kHz

3 to 30 us PULSE WIDTH

PULSE GENERATOR

SERIAL NUMBER: _____

WARRANTY

Avtech Electrosystems Ltd. warrants products of its manufacture to be free from defects in material and workmanship under conditions of normal use. If, within one year after delivery to the original owner, and after prepaid return by the original owner, this Avtech product is found to be defective, Avtech shall at its option repair or replace said defective item. This warranty does not apply to units which have been disassembled, modified or subjected to conditions exceeding the applicable specifications or ratings. This warranty is the extent of the obligation assumed by Avtech with respect to this product and no other warranty or guarantee is either expressed or implied.

TECHNICAL SUPPORT

Phone: 888-670-8729 (USA & Canada) or +1-613-226-5772 (Intl)

Fax: 800-561-1970 (USA & Canada) or +1-613-226-2802 (Intl)

E-mail: info@avtechpulse.com

World Wide Web: <http://www.avtechpulse.com>

TABLE OF CONTENTS

WARRANTY.....	2
TECHNICAL SUPPORT.....	2
TABLE OF CONTENTS.....	3
INTRODUCTION.....	5
SPECIFICATIONS.....	6
EUROPEAN REGULATORY NOTES.....	7
EC DECLARATION OF CONFORMITY.....	7
DIRECTIVE 2002/95/EC (RoHS).....	7
DIRECTIVE 2002/96/EC (WEEE).....	7
INSTALLATION.....	9
VISUAL CHECK.....	9
POWER RATINGS.....	9
CONNECTION TO THE POWER SUPPLY.....	9
PROTECTION FROM ELECTRIC SHOCK.....	10
ENVIRONMENTAL CONDITIONS.....	10
FUSES.....	12
AC FUSE REPLACEMENT.....	12
DC FUSE REPLACEMENT.....	13
FUSE RATINGS.....	13
FRONT PANEL CONTROLS.....	14
REAR PANEL CONTROLS.....	16
GENERAL INFORMATION.....	17
BASIC TEST ARRANGEMENT.....	17
BASIC PULSE CONTROL.....	17
LOAD IMPEDANCE.....	19
OUTPUT IMPEDANCE.....	19
MECHANICAL INFORMATION.....	20
TOP COVER REMOVAL.....	20
RACK MOUNTING.....	20
ELECTROMAGNETIC INTERFERENCE.....	20
MAINTENANCE.....	21
REGULAR MAINTENANCE.....	21

CLEANING.....	21
<i>WIRING DIAGRAMS.....</i>	22
WIRING OF AC POWER.....	22
PCB 158K - LOW VOLTAGE POWER SUPPLY, 1/3.....	23
PCB 158K - LOW VOLTAGE POWER SUPPLY, 2/3.....	24
PCB 158K - LOW VOLTAGE POWER SUPPLY, 3/3.....	25
PCB 168B - HIGH VOLTAGE DC POWER SUPPLY.....	26
PCB 80B - TIMING BOARD (1/2).....	27
PCB 80B - TIMING BOARD (2/2).....	28
MAIN WIRING.....	29
<i>PERFORMANCE CHECK SHEET.....</i>	30

Manual Reference: T:\instructword\avr-g\AVR-G1-C-EMRA, edition 8.odt.
Last modified July 25, 2006.
Copyright © 2006 Avtech Electrosystems Ltd, All Rights Reserved.

INTRODUCTION

The AVR-G1-C-EMRA-P is a high performance instrument capable of generating up to +240V (into $R_L \geq 1.6 \text{ k}\Omega$, 150 mA maximum, $C_L \leq 900 \text{ pF}$) at repetition rates up to 10 kHz. The output pulse width is variable from 3 to 30 μs . The rise time is less than 10 ns, and the fall time is less than 20 ns.

This instrument is intended for use in research and development laboratories.

SPECIFICATIONS

Model:	AVR-G1-C-EMRA-P
Amplitude:	0 to +240 Volts
Pulse width:	3 to 30 us
Load impedance:	$R_L \geq 1.6 \text{ k}\Omega$, 150 mA maximum, $C_L \leq 900 \text{ pF}$
Rise time:	$\leq 10 \text{ ns}$ (for a resistive load)
Fall time:	$\leq 20 \text{ ns}$ (for a resistive load)
PRF:	1 to 10 kHz
Polarity:	Positive
Propagation delay:	$\leq 100 \text{ ns}$ (Ext trig in to pulse out)
Jitter (Ext trig in to pulse out):	$\pm 100 \text{ ps} \pm 0.03\%$ of sync delay
Trigger required: (ext trig mode)	Mode A: + 5 Volt, 50 ns - 500 ns (TTL) Mode B: + 5 Volt, $PW_{IN} = PW_{OUT}$ (TTL)
Sync delay:	Variable, 0 to $\pm 30 \text{ us}$
Sync output:	+ 3 Volts, 200 ns, will drive 50 Ohm loads
Monitor output:	The rear panel M BNC connector provides DC output voltage (to $R_L \geq 1 \text{ M}\Omega$) which is proportional to the peak load current (33 mV/mA). For a peak load current of 150 mA, the output will be +5.0 Volts.
Connectors:	Out, Trig: BNC
Power requirements:	100 - 240 Volts, 50-60 Hz
Dimensions (H x W x D):	100 mm x 430 mm x 375 mm (3.9" x 17" x 14.8")
Chassis material:	cast aluminum frame and handles, blue vinyl on aluminum cover plates
Mounting:	Any
Temperature range:	+5°C to +40°C

EUROPEAN REGULATORY NOTES

EC DECLARATION OF CONFORMITY

We Avtech Electrosystems Ltd.
 P.O. Box 5120, LCD Merivale
 Ottawa, Ontario
 Canada K2C 3H4

declare that this pulse generator meets the intent of Directive 89/336/EEC for Electromagnetic Compatibility. Compliance pertains to the following specifications as listed in the official Journal of the European Communities:

EN 50081-1 Emission

EN 50082-1 Immunity

and that this pulse generator meets the intent of the Low Voltage Directive 72/23/EEC as amended by 93/68/EEC. Compliance pertains to the following specifications as listed in the official Journal of the European Communities:

EN 61010-1:2001 Safety requirements for electrical equipment for measurement, control, and laboratory use



DIRECTIVE 2002/95/EC (RoHS)

This instrument is exempt from Directive 2002/95/EC of the European Parliament and of the Council of 27 January 2003 on the Restriction of the use of certain Hazardous Substances (RoHS) in electrical and electronic equipment. Specifically, Avtech instruments are considered "Monitoring and control instruments" (Category 9) as defined in Annex 1A of Directive 2002/96/EC. The Directive 2002/95/EC only applies to Directive 2002/96/EC categories 1-7 and 10, as stated in the "Article 2 - Scope" section of Directive 2002/95/EC.

DIRECTIVE 2002/96/EC (WEEE)

European customers who have purchased this equipment directly from Avtech will have completed a "WEEE Responsibility Agreement" form, accepting responsibility for

WEEE compliance (as mandated in Directive 2002/96/EC of the European Union and local laws) on behalf of the customer, as provided for under Article 9 of Directive 2002/96/EC.

Customers who have purchased Avtech equipment through local representatives should consult with the representative to determine who has responsibility for WEEE compliance. Normally, such responsibilities will lie with the representative, unless other arrangements (under Article 9) have been made.

Requirements for WEEE compliance may include registration of products with local governments, reporting of recycling activities to local governments, and financing of recycling activities.



INSTALLATION

VISUAL CHECK

After unpacking the instrument mainframe and the transformer module, examine to ensure that they have not been damaged in shipment. Visually inspect all connectors, knobs, and handles. Confirm that a power cord and an instrumentation manual (this manual), are with the instrument. If the instrument has been damaged, file a claim immediately with the company that transported the instrument.

POWER RATINGS

This instrument is intended to operate from 100 - 240 V, 50 - 60 Hz.

The maximum power consumption is 74 Watts. Please see the "FUSES" section for information about the appropriate AC and DC fuses.

This instrument is an "Installation Category II" instrument, intended for operation from a normal single-phase supply.

CONNECTION TO THE POWER SUPPLY

An IEC-320 three-pronged recessed male socket is provided on the back panel for AC power connection to the instrument. One end of the detachable power cord that is supplied with the instrument plugs into this socket. The other end of the detachable power cord plugs into the local mains supply. Use only the cable supplied with the instrument. The mains supply must be earthed, and the cord used to connect the instrument to the mains supply must provide an earth connection. (The supplied cord does this.)

 **Warning:** Failure to use a grounded outlet may result in injury or death due to electric shock. This product uses a power cord with a ground connection. It must be connected to a properly grounded outlet. The instrument chassis is connected to the ground wire in the power cord.

The table below describes the power cord that is normally supplied with this instrument, depending on the destination region:

Destination Region	Description	Manufacturer	Part Number
Continental Europe	European CEE 7/7 "Schuko" 230V, 50Hz	Volex (http://www.volex.com)	17850-C3-326
United Kingdom	BS 1363, 230V, 50Hz	Volex (http://www.volex.com)	17962-C3-10
Switzerland	SEV 1011, 230V, 50Hz	Volex (http://www.volex.com)	2102H-C3-10
Israel	SI 32, 220V, 50Hz	Volex (http://www.volex.com)	2115H-C3-10
North America, and all other areas	NEMA 5-15, 120V, 60 Hz	Volex (http://www.volex.com)	17250-B1-10
		Qualtek (http://www.qualtekusa.com)	312007-01

PROTECTION FROM ELECTRIC SHOCK

 Operators of this instrument must be protected from electric shock at all times. The owner must ensure that operators are prevented access and/or are insulated from every connection point. In some cases, connections must be exposed to potential human contact. Operators must be trained to protect themselves from the risk of electric shock. This instrument is intended for use by qualified personnel who recognize shock hazards and are familiar with safety precautions required to avoid possibly injury. In particular, operators should:

1. Keep exposed high-voltage wiring to an absolute minimum.
2. Wherever possible, use shielded connectors and cabling.
3. Connect and disconnect loads and cables only when the instrument is turned off.
4. Keep in mind that all cables, connectors, oscilloscope probes, and loads must have an appropriate voltage rating.
5. Do not attempt any repairs on the instrument, beyond the fuse replacement procedures described in this manual. Contact Avtech technical support (see page 2 for contact information) if the instrument requires servicing. Service is to be performed solely by qualified service personnel.

ENVIRONMENTAL CONDITIONS


This instrument is intended for use under the following conditions:

1. indoor use;
2. altitude up to 2 000 m;
3. temperature 5 °C to 40 °C;
4. maximum relative humidity 80 % for temperatures up to 31 °C decreasing linearly to 50 % relative humidity at 40 °C;
5. Mains supply voltage fluctuations up to ± 10 % of the nominal voltage;

6. no pollution or only dry, non-conductive pollution.


FUSES

This instrument contains four fuses. All are accessible from the rear-panel. Two protect the AC prime power input, and two protect the internal DC power supplies. The locations of the fuses on the rear panel are shown in the figure below:

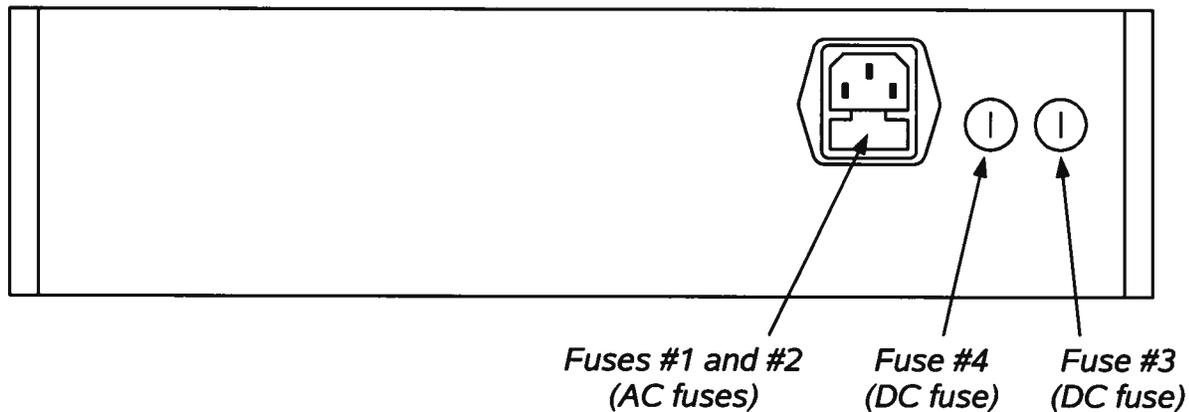

AC FUSE REPLACEMENT

To physically access the AC fuses, the power cord must be detached from the rear panel of the instrument. The fuse drawer may then be extracted using a small flat-head screwdriver, as shown below:

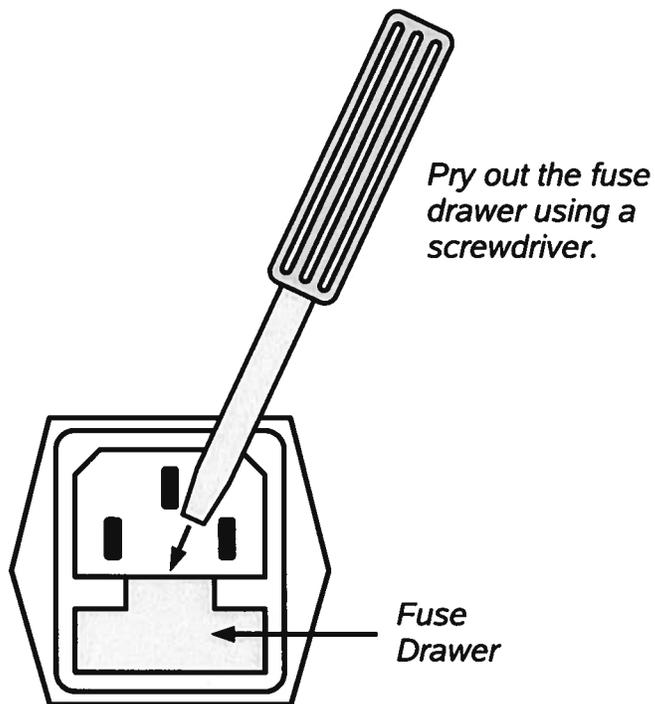

DC FUSE REPLACEMENT

The DC fuses may be replaced by inserting the tip of a flat-head screwdriver into the fuse holder slot, and rotating the slot counter-clockwise. The fuse and its carrier will then pop out.

FUSE RATINGS


The following table lists the required fuses:

Fuses	Nominal Mains Voltage	Rating	Case Size	Recommended Replacement Part	
				Littelfuse Part Number	Digi-Key Stock Number
#1, #2 (AC)	100-240V	0.5A, 250V, Time-Delay	5×20 mm	0218.500HXP	F2416-ND
#3 (DC)	N/A	1.6A, 250V, Time-Delay	5×20 mm	021801.6HXP	F2424-ND
#4 (DC)	N/A	0.8A, 250V, Time-Delay	5×20 mm	0218.800HXP	F2418-ND

The recommended fuse manufacturer is Littelfuse (<http://www.littelfuse.com>).

Replacement fuses may be easily obtained from Digi-Key (<http://www.digikey.com>) and other distributors.

FRONT PANEL CONTROLS

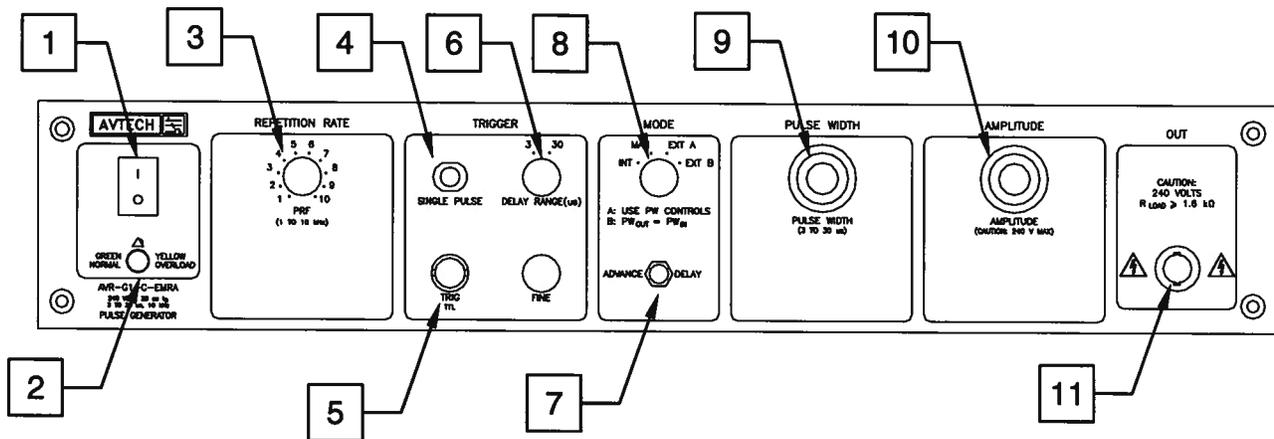

1. **POWER Switch**. This is the main power switch. When turning the instrument on, there may be a delay of several seconds before the instrument appears to respond.
2. **OVERLOAD Indicator**. When the instrument is powered, this indicator is normally green, indicating normal operation. If this indicator is yellow, an internal automatic overload protection circuit has been tripped. If the unit is overloaded (by operating at an exceedingly high duty cycle or by operating into a very low impedance), the protective circuit will disable the output of the instrument and turn the indicator light yellow. The light will stay yellow (i.e. output disabled) for about 5 seconds after which the instrument will attempt to re-enable the output (i.e. light green) for about 1 second. If the overload condition persists, the output will be disabled again (i.e. light yellow) for another 5 seconds. If the overload condition has been removed, the instrument will resume normal operation.

This overload indicator may flash yellow briefly at start-up. This is not a cause for concern.

3. **PRF Range Switch and Vernier**. This switch sets the pulse repetition frequency (PRF) range of the internal oscillator. The marked value of each position is the upper limit of the range, approximately. The vernier dial directly below the switch varies the PRF within the set range.
4. **SINGLE PULSE Push Button**. The "SINGLE PULSE" push button will trigger the instrument manually for one cycle of output, when the "MODE" switch is in the "MAN" position. Otherwise, the push button has no effect.
5. **TRIG Connector**. When the "MODE" switch is in the "EXT" position, this connector is an input. The external trigger (50 ns or wider, TTL levels) is applied to this connector.

When operating in the "INT" mode, this connector is an output. A SYNC output is generated on this connector, to synchronize oscilloscopes or other measurement

systems.

6. Delay Range Switch and Vernier. This switch and one-turn dial sets the delay between the main output and the TRIG output. The marked value of each switch position is the upper limit of the range, approximately. The vernier dial directly below the switch varies the delay within the set range.
7. ADVANCE/DELAY Switch. With this switch in the DELAY position, the leading edge of the output pulse precedes the leading edge of the TRIG output. When in the ADVANCE position, the leading edge of the TRIG output precedes the leading edge of the main output.
8. MODE Switch. In the "INT" position the instrument is internally triggered and the TRIG connector provides a SYNC output which allows one to trigger other instruments, such as oscilloscopes.

In the "MAN" position a single pulse can be generated by pressing the "SINGLE PULSE" push button. The TRIG connector is not used in this mode.


In the "EXT A" position the instrument is triggered by a TTL-level pulse on the TRIG connector. The output parameters (pulse width, delay, and amplitude) are determined by the front panel settings.

In the "EXT B" position the instrument is triggered by a TTL-level pulse on the TRIG connector. The output pulse occurs with nominally zero delay, and the output pulse width is approximately equal to the input pulse width. The amplitude is controlled by the front panel settings.

9. PULSE WIDTH Controls. This switch and ten-turn dial set the pulse width of the the main output. The marked value of each switch position is the upper limit of the range, approximately. The vernier dial directly below the switch varies the delay within the set range.
10. AMPLITUDE Controls. This ten-turn dial provides continuously variable control of the peak amplitude of the main output from 0 to the full-scale range value.
11. OUT CONNECTOR. This BNC connector provides the main output signal, into load impedances of $R_L \geq 1.6 \text{ k}\Omega$ (150 mA maximum), $C_L \leq 900 \text{ pF}$.

 Caution: Voltages as high as 240V may be present on the center conductor of this output connector. Avoid touching this conductor. Connect to this connector using standard coaxial cable, to ensure that the center conductor is not exposed.

REAR PANEL CONTROLS

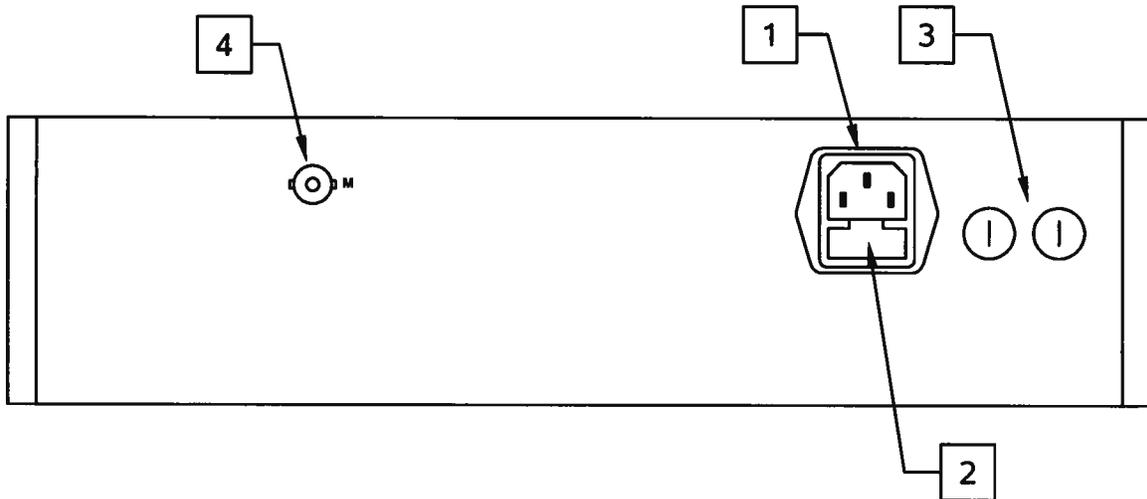


1. AC POWER INPUT. An IEC-320 C14 three-pronged recessed male socket is provided on the back panel for AC power connection to the instrument. One end of the detachable power cord that is supplied with the instrument plugs into this socket.
2. AC FUSE DRAWER. The two fuses that protect the AC input are located in this drawer. Please see the “FUSES” section of this manual for more information.
3. DC FUSES. These two fuses protect the internal DC power supplies. Please see the “FUSES” sections of this manual for more information.
4. MONITOR Output. The rear panel M BNC connector provides DC output voltage (to $R_L \geq 1 \text{ M}\Omega$) which is proportional to the peak load current (33 mV/mA). For a peak load current of 150 mA, the output will be +5.0 Volts.

GENERAL INFORMATION

BASIC TEST ARRANGEMENT

The AVR-G1-C-EMRA should be tested with a sampling oscilloscope with a bandwidth of at least 100 MHz to properly observe the high-speed waveform. A typical test arrangement is shown below:

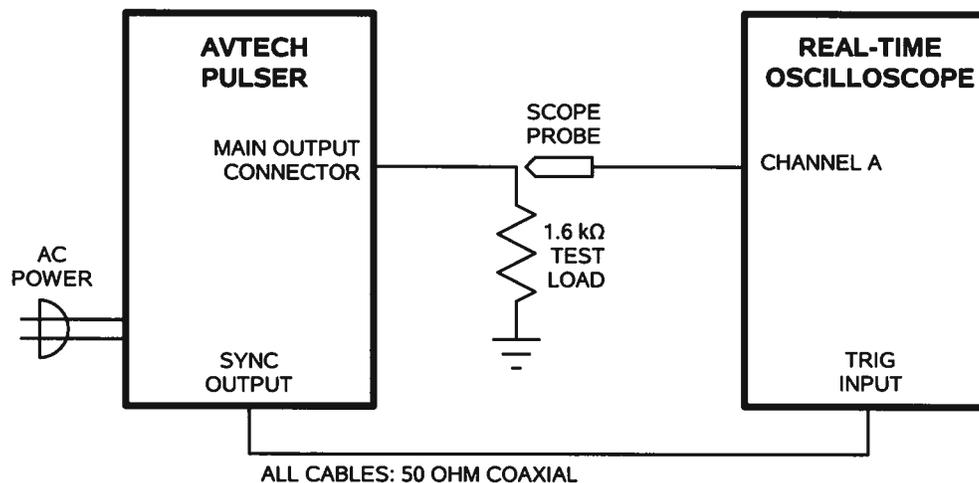


BASIC PULSE CONTROL


This instrument can be triggered by its own internal clock or by an external TTL trigger signal. When triggered internally, two mainframe output channels respond to the trigger: OUT and SYNC.

- OUT. This is the main output. The maximum output voltage is 240V.
- TRIG. The TRIG pulse is a fixed-width TTL-level reference pulse used to trigger oscilloscopes or other measurement systems.


When the ADVANCE/DELAY switch is set to "ADVANCE", the TRIG output precedes the main output. These pulses are illustrated below:

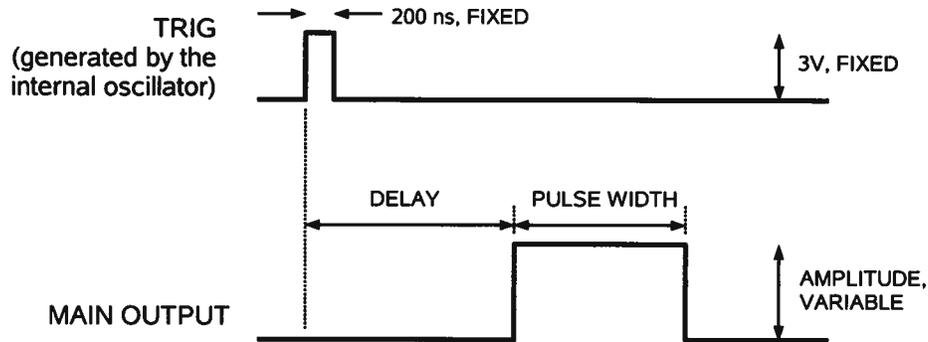


When the ADVANCE/DELAY switch is set to "DELAY", the TRIG output occurs after the main output. This illustrated below:

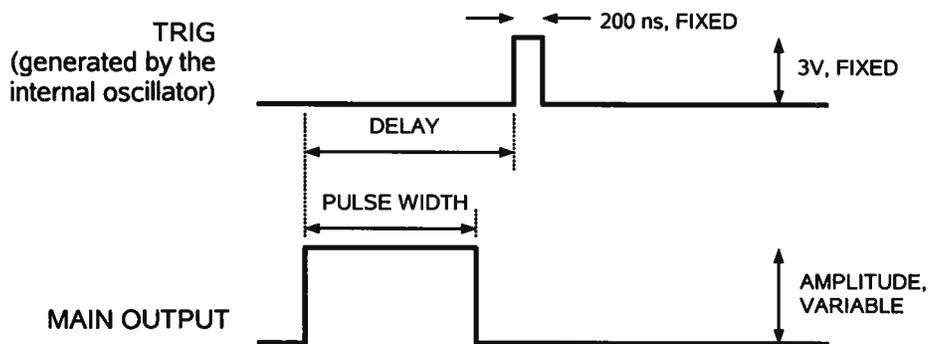

When triggered externally, the TRIG connector acts as an input. In the EXT A mode, the output parameters (pulse width, delay, and amplitude) are determined by the front panel settings. This is illustrated below:

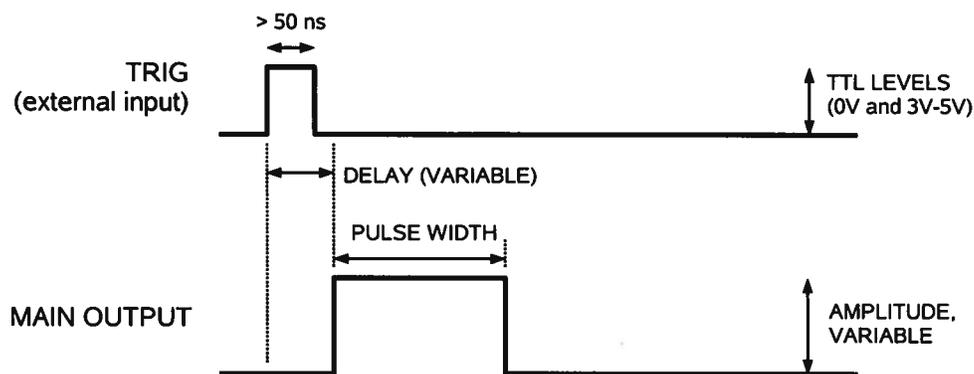

In the "EXT B" mode the instrument is triggered by a TTL-level pulse on the TRIG connector. The output pulse occurs with nominally zero delay, and the output pulse width is approximately equal to the input pulse width. The amplitude is controlled by the front panel settings. This is illustrated below:

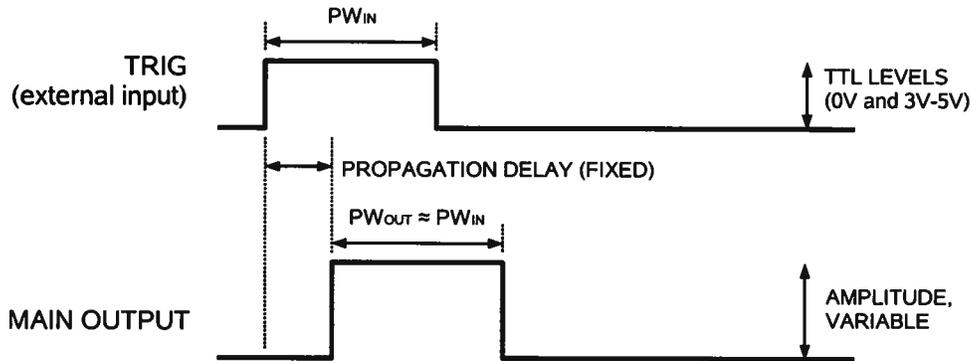

LOAD IMPEDANCE

⚠ This unit was specifically designed to drive high impedance loads ($R_L \geq 1.6 \text{ k}\Omega$, 150 mA maximum, $C_L \leq 900 \text{ pF}$). The unit may fail if operated into low impedance loads (e.g. 50Ω).

OUTPUT IMPEDANCE

The output impedance of the pulser may be varied between 5Ω and 50Ω by varying the value of the 2 Watt resistor on the carrier PCB on the output of the -PG module. The unit was shipped with a 50Ω resistor in place. The higher the value of the resistor, the longer the rise-fall time. The resistor may be accessed by removing the four Philips screws on the top panel. The top cover may then be slid back and off.

MECHANICAL INFORMATION

TOP COVER REMOVAL

If necessary, the interior of the instrument may be accessed by removing the four Phillips screws on the top panel. With the four screws removed, the top cover may be slid back (and off).

 Always disconnect the power cord and allow the instrument to sit unpowered for 10 minutes before opening the instrument. This will allow any internal stored charge to discharge.

There are no user-adjustable internal circuits. For repairs other than fuse replacement, please contact Avtech (info@avtechpulse.com) to arrange for the instrument to be returned to the factory for repair. Service is to be performed solely by qualified service personnel.

 Caution: High voltages are present inside the instrument during normal operation. Do not operate the instrument with the cover removed.

RACK MOUNTING

A rack mounting kit is available. The -R5 rack mount kit may be installed after first removing the one Phillips screw on the side panel adjacent to the front handle.

ELECTROMAGNETIC INTERFERENCE

To prevent electromagnetic interference with other equipment, all used outputs should be connected to shielded loads using shielded coaxial cables. Unused outputs should be terminated with shielded coaxial terminators or with shielded coaxial dust caps, to prevent unintentional electromagnetic radiation. All cords and cables should be less than 3m in length.

MAINTENANCE

REGULAR MAINTENANCE


This instrument does not require any regular maintenance.

On occasion, one or more of the four rear-panel fuses may require replacement. All fuses can be accessed from the rear panel. See the “FUSES” section for details.

CLEANING



If desired, the interior of the instrument may be cleaned using compressed air to dislodge any accumulated dust. (See the “TOP COVER REMOVAL” section for instructions on accessing the interior.) No other cleaning is recommended.

PCB 158K - LOW VOLTAGE POWER SUPPLY, 2/3

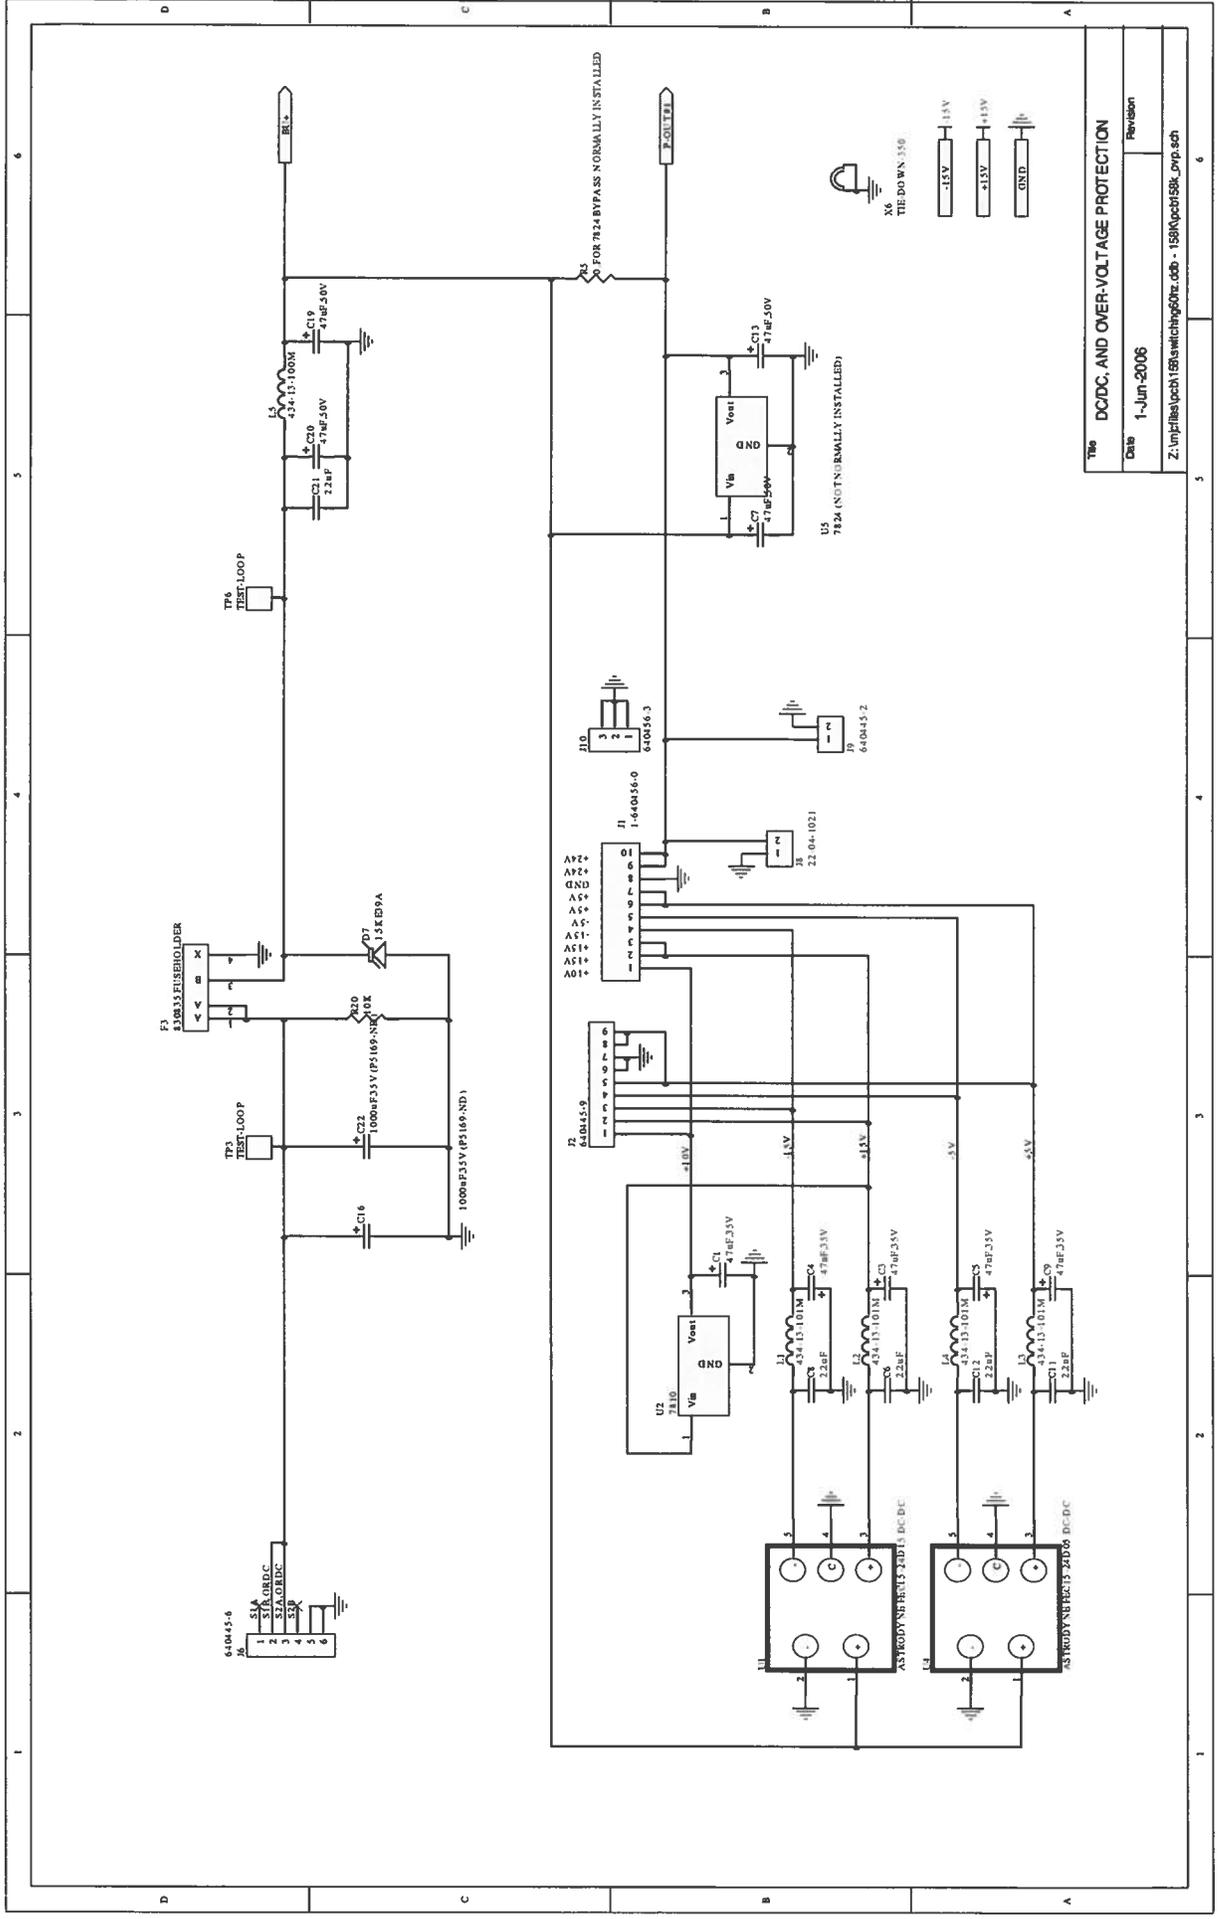



Title		DC/DC, AND OVER-VOLTAGE PROTECTION
Date	1-Jun-2006	
Revision	1	
Z:\mpj\Bas\pcc\158k\switching60hz.dcb - 158k\pcb158k_omp.sch		

PCB 158K - LOW VOLTAGE POWER SUPPLY, 3/3

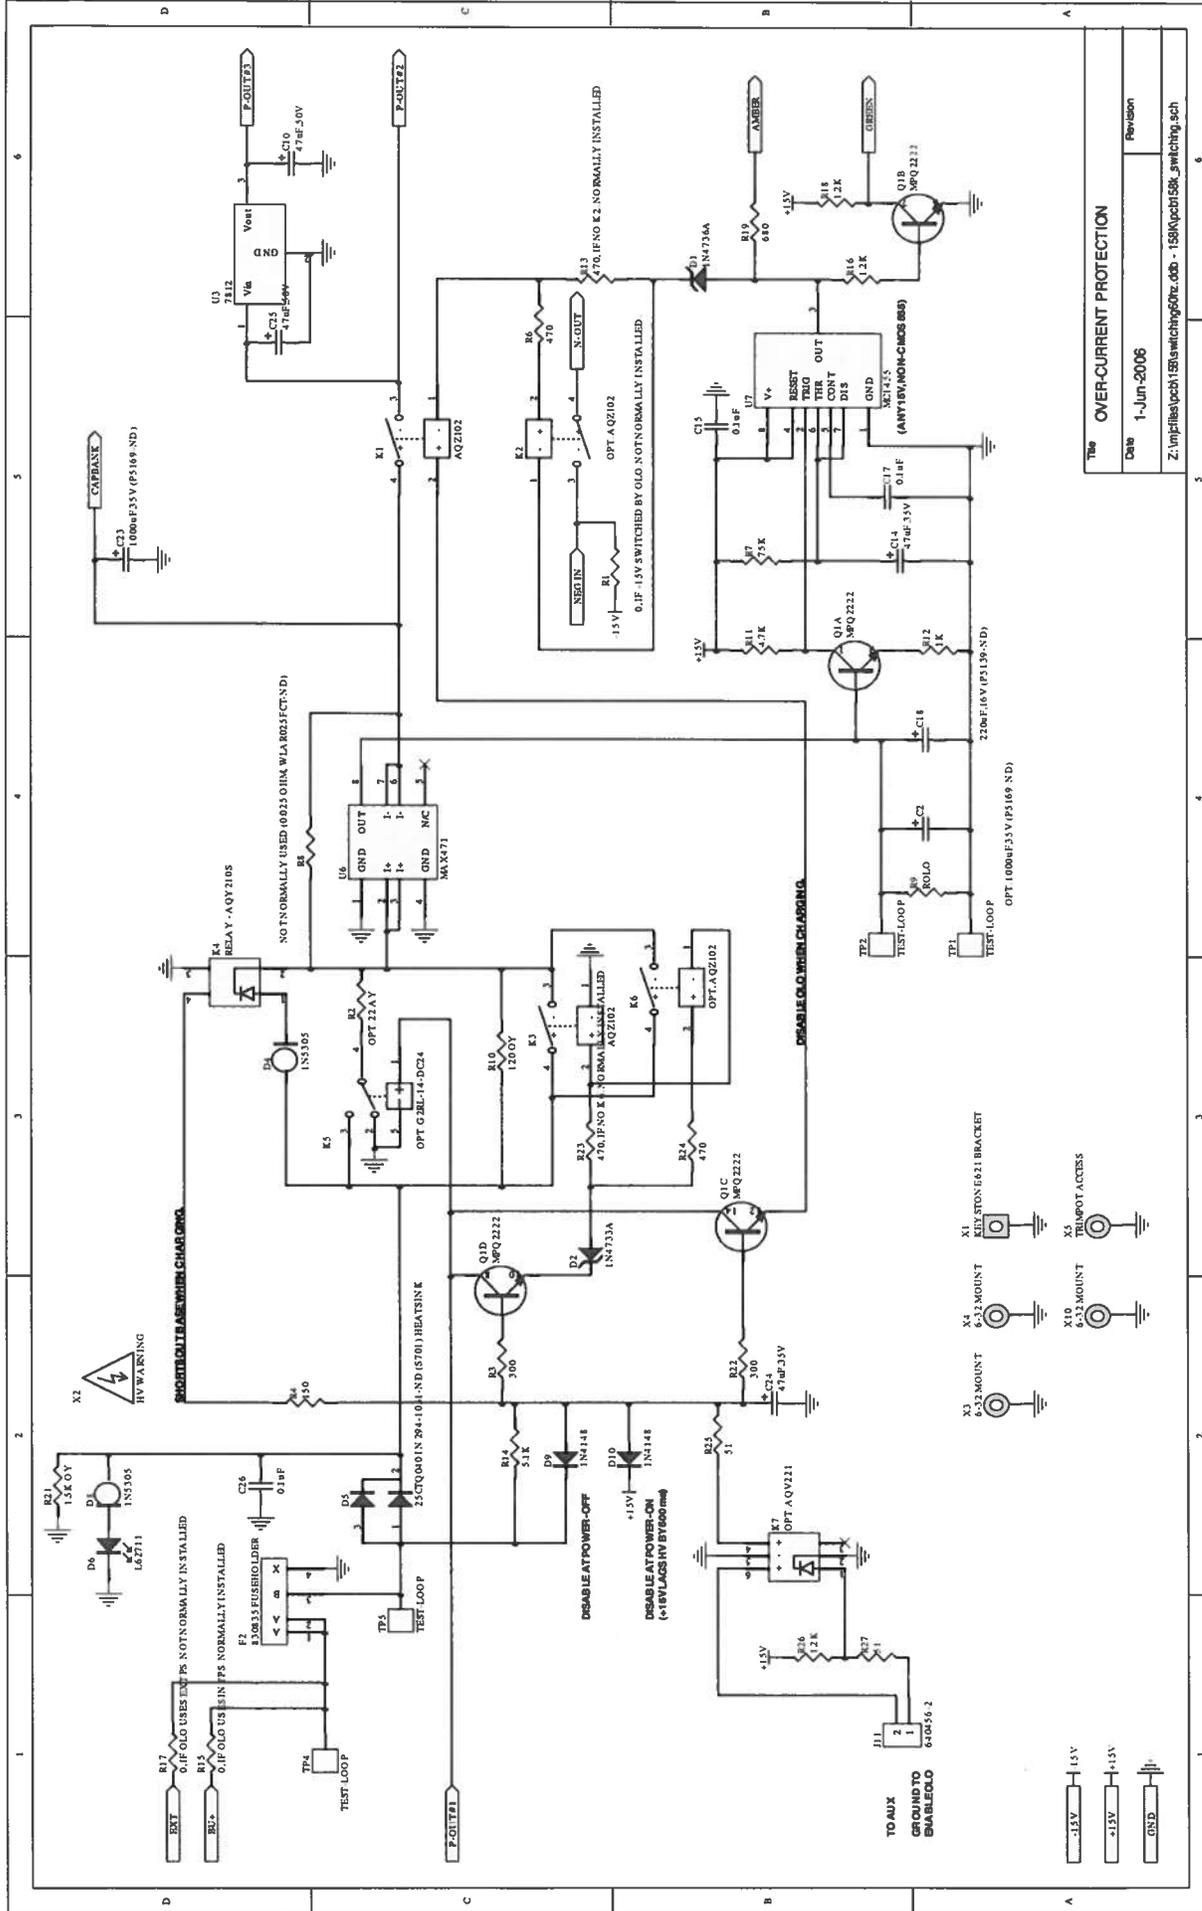


The OVERCURRENT PROTECTION
 Date 1-Jun-2006
 Revision
 Z:\mp\files\pch158k\switching60hz.dcb - t:150k\pcht158k_switching.sch

PCB 168B - HIGH VOLTAGE DC POWER SUPPLY

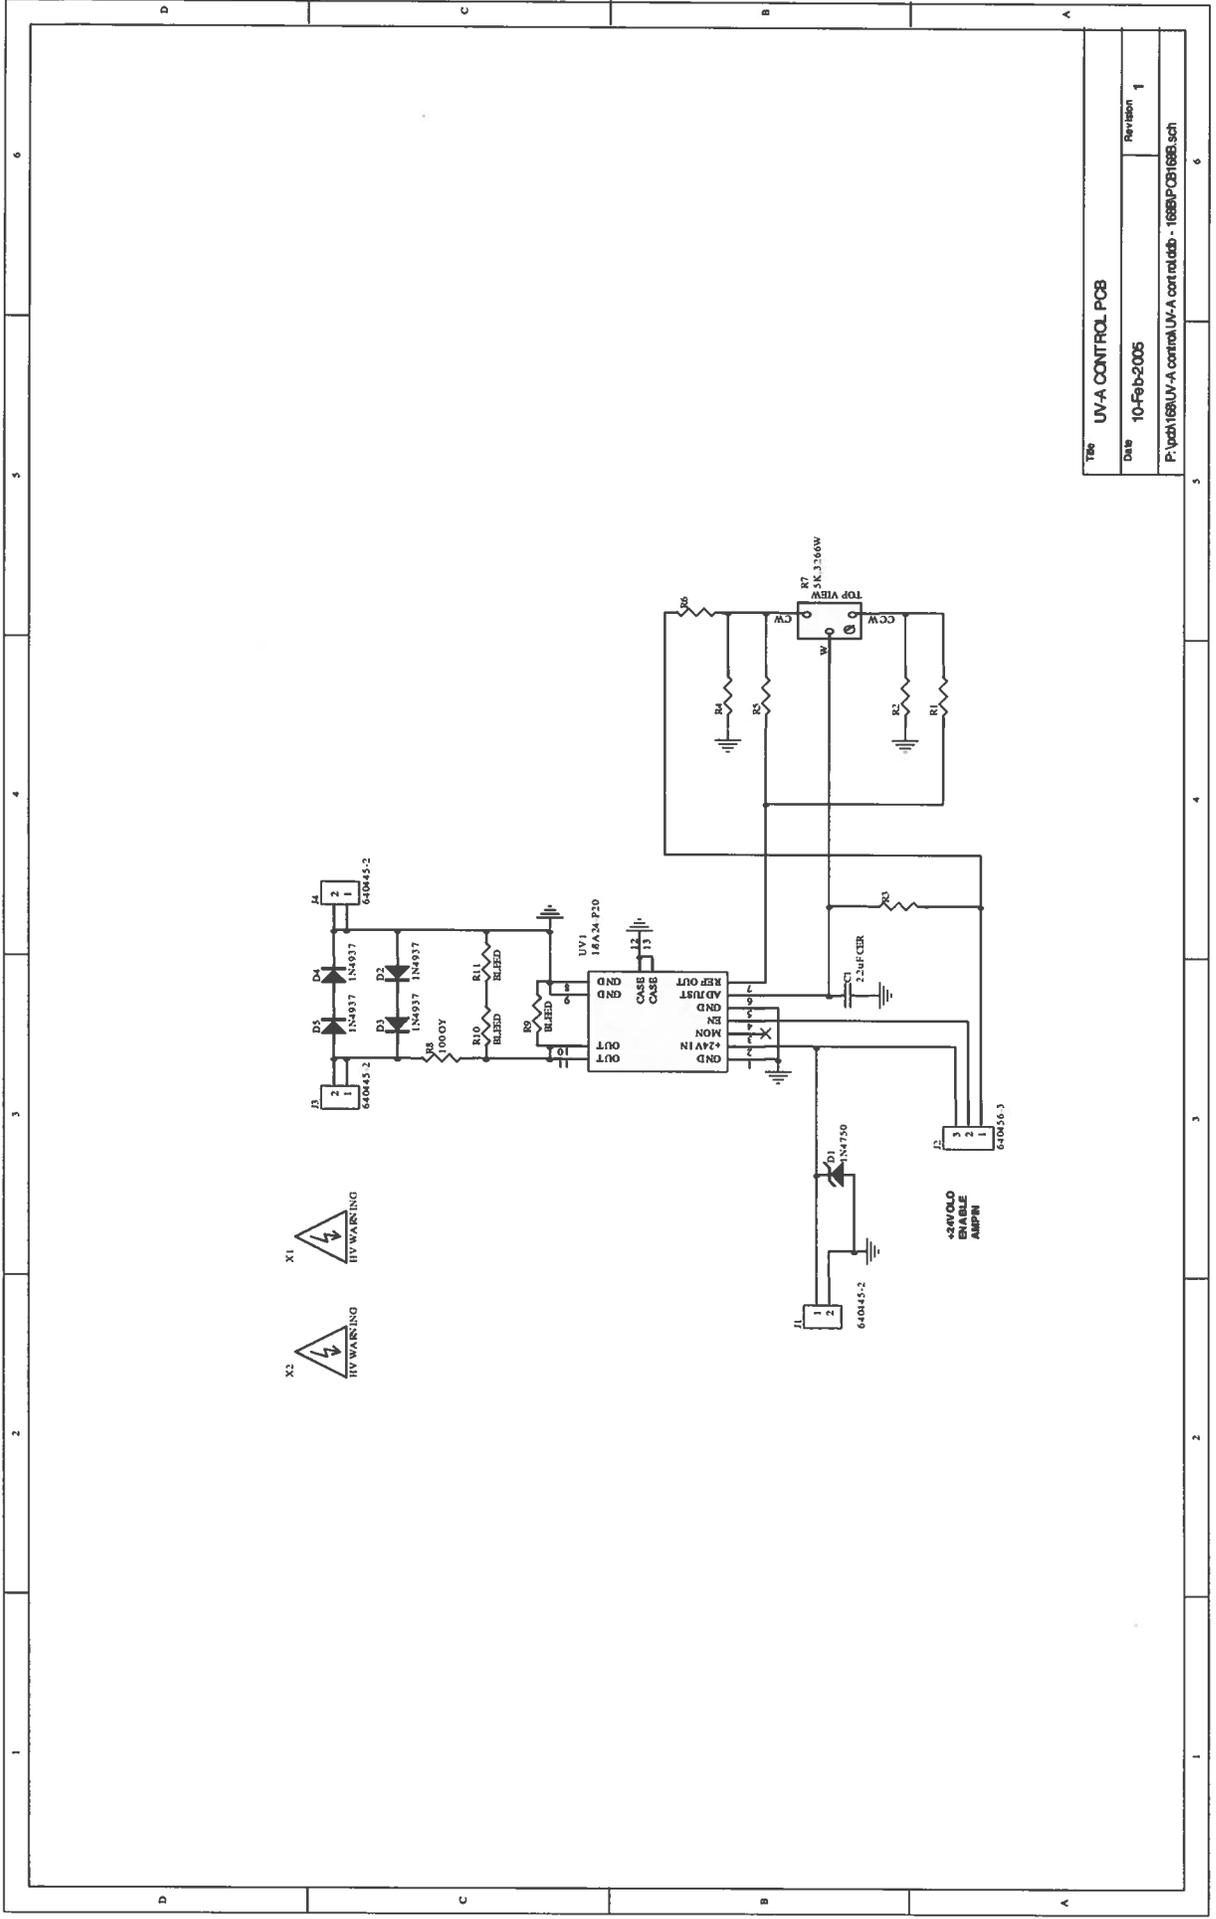



Tab UV-A CONTROL PCB
 Date 10-Feb-2005
 Revision 1
 P:\pcb\168UV-A control UV-A control.ddb - 168BPCB168B.sch

PCB 80B - TIMING BOARD (1/2)

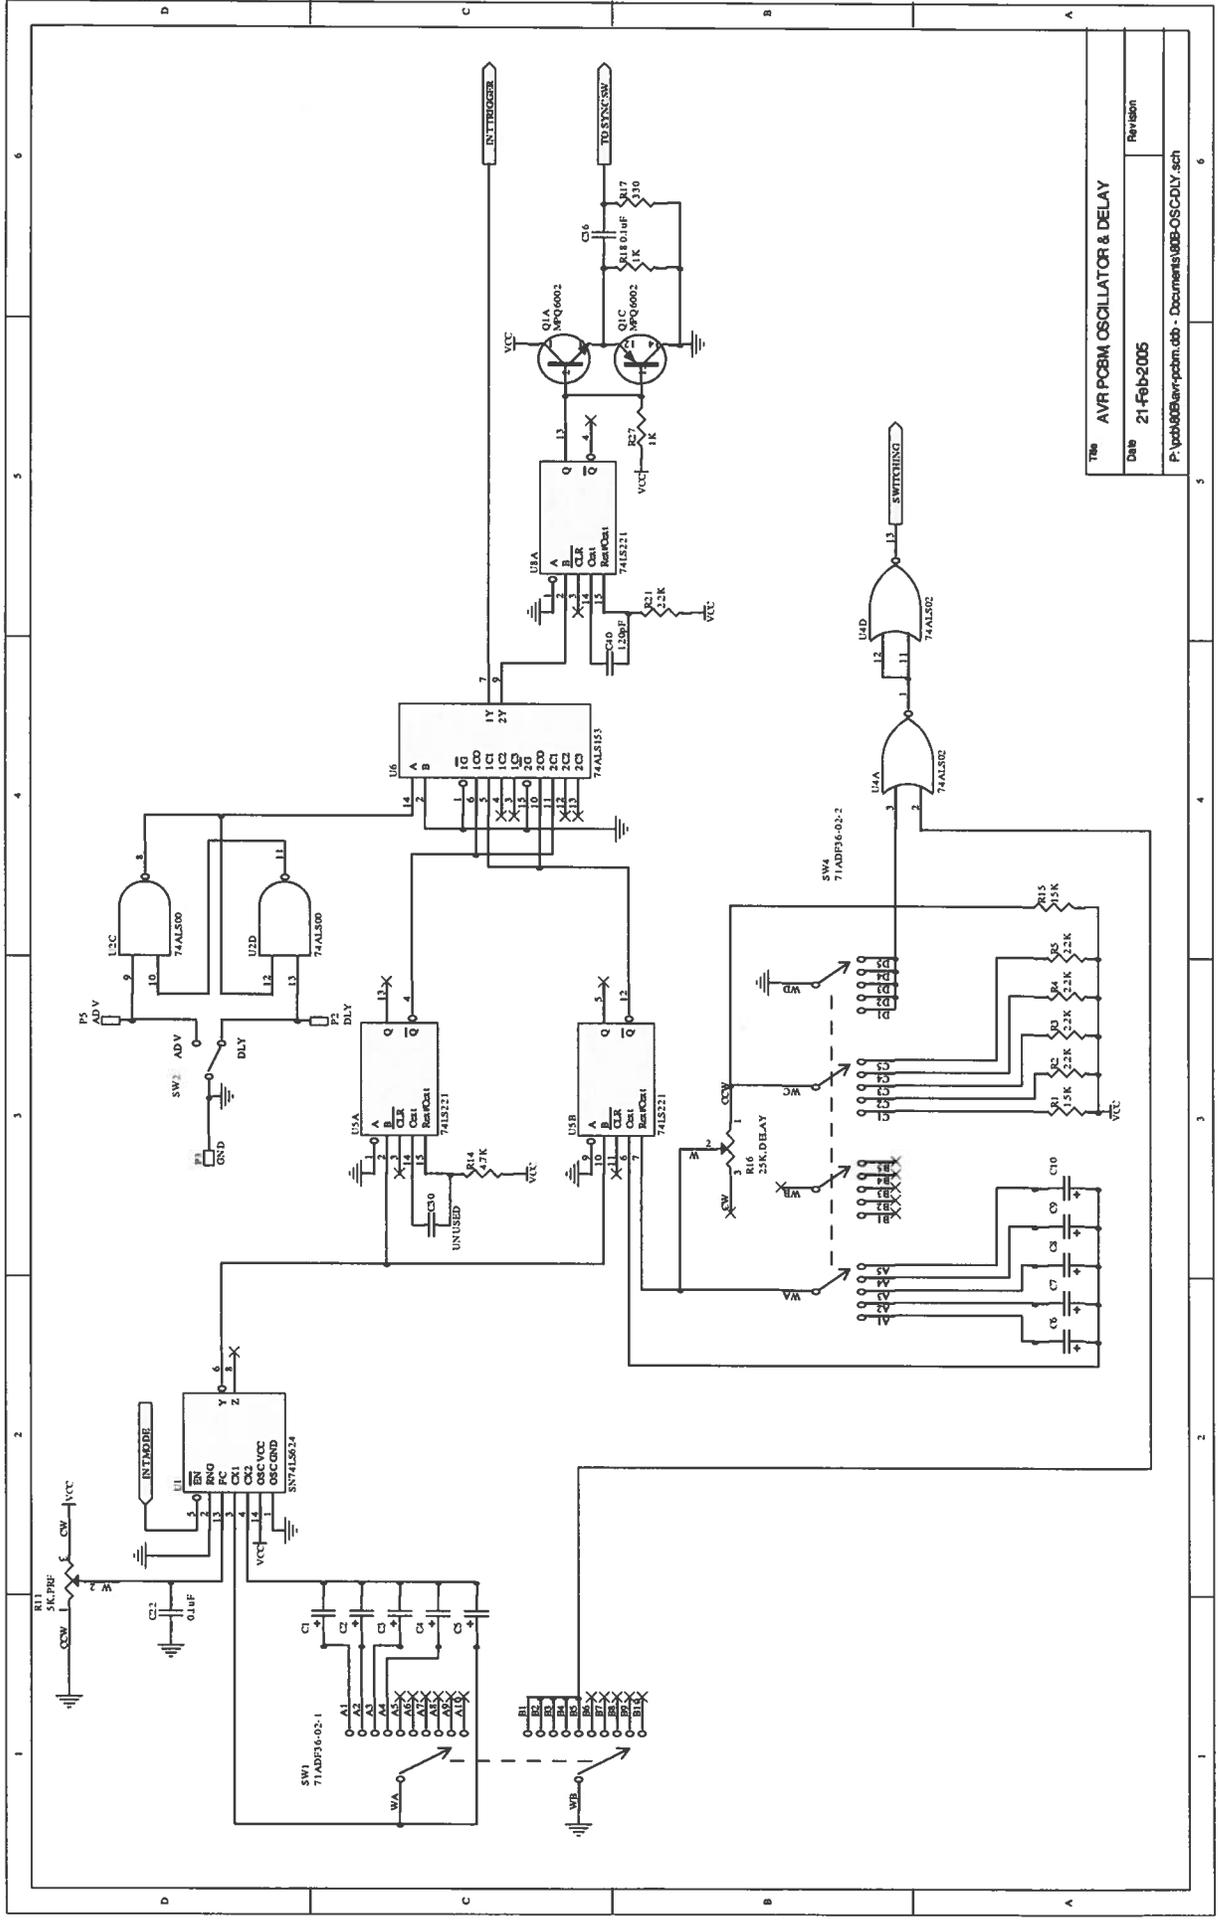

Title	AVR PCB8M OSCILLATOR & DELAY
Date	21-Feb-2005
Revision	
P:\pcb80B\avr-pcbm.ddb - Documents\80B-OSC.DLY.sch	

PCB 80B - TIMING BOARD (2/2)

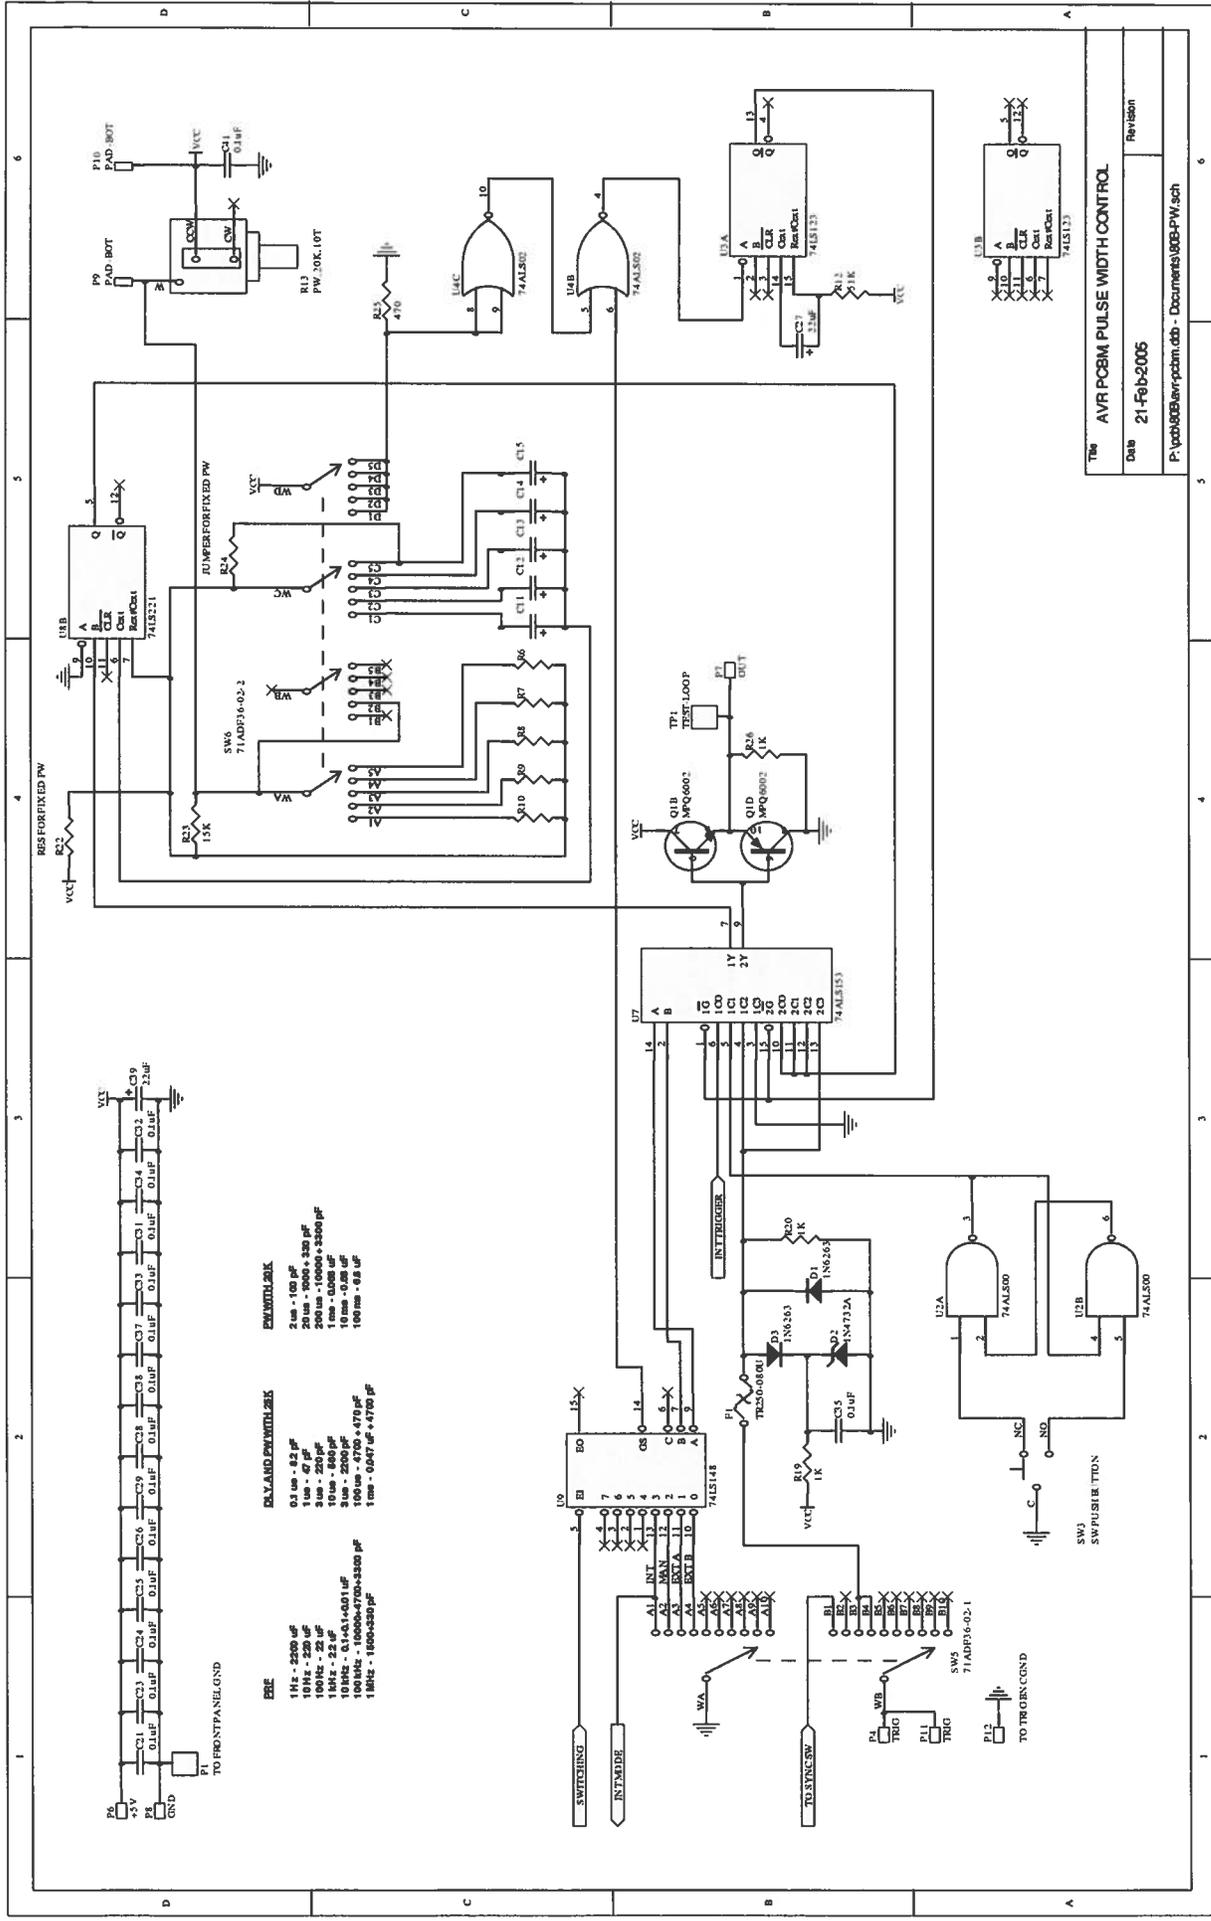

RESFORMER PW

DELAY AND PW NETWORKS

5ms - 100 pF	5ms - 100 pF
20ms - 1000 pF	10ms - 1000 pF
100ms - 10000 pF	100ms - 10000 pF
200ms - 100000 pF	10ms - 10000 pF
1ms - 0.001 uF	10ms - 0.001 uF
10ms - 0.01 uF	100ms - 0.01 uF
100ms - 0.1 uF	1ms - 0.001 uF
1ms - 0.001 uF	1ms - 0.001 uF

FW NETWORKS

5ms - 100 pF	5ms - 100 pF
20ms - 1000 pF	10ms - 1000 pF
100ms - 10000 pF	100ms - 10000 pF
200ms - 100000 pF	10ms - 10000 pF
1ms - 0.001 uF	10ms - 0.001 uF
10ms - 0.01 uF	100ms - 0.01 uF
100ms - 0.1 uF	1ms - 0.001 uF
1ms - 0.001 uF	1ms - 0.001 uF

DELTA AND PW NETWORKS

0.1ms - 0.5 pF	0.1ms - 0.5 pF
1ms - 5 pF	1ms - 5 pF
10ms - 50 pF	10ms - 50 pF
100ms - 500 pF	100ms - 500 pF
1ms - 5 nF	1ms - 5 nF
10ms - 50 nF	10ms - 50 nF
100ms - 500 nF	100ms - 500 nF
1ms - 5 uF	1ms - 5 uF
10ms - 50 uF	10ms - 50 uF
100ms - 500 uF	100ms - 500 uF
1ms - 5 mF	1ms - 5 mF

SWITCHING

SW1	SW2	SW3	SW4	SW5
SW6	SW7	SW8	SW9	SW10
SW11	SW12	SW13	SW14	SW15
SW16	SW17	SW18	SW19	SW20
SW21	SW22	SW23	SW24	SW25

TEST POINTS

TP1	TP2	TP3	TP4	TP5
TP6	TP7	TP8	TP9	TP10
TP11	TP12	TP13	TP14	TP15
TP16	TP17	TP18	TP19	TP20
TP21	TP22	TP23	TP24	TP25

RESISTORS

R1	R2	R3	R4	R5
R6	R7	R8	R9	R10
R11	R12	R13	R14	R15
R16	R17	R18	R19	R20
R21	R22	R23	R24	R25

CAPACITORS

C1	C2	C3	C4	C5
C6	C7	C8	C9	C10
C11	C12	C13	C14	C15
C16	C17	C18	C19	C20
C21	C22	C23	C24	C25

ICs

U1	U2	U3	U4	U5
U6	U7	U8	U9	U10
U11	U12	U13	U14	U15
U16	U17	U18	U19	U20
U21	U22	U23	U24	U25

DIODES

D1	D2	D3	D4	D5
D6	D7	D8	D9	D10
D11	D12	D13	D14	D15
D16	D17	D18	D19	D20
D21	D22	D23	D24	D25

TRANSISTORS

T1	T2	T3	T4	T5
T6	T7	T8	T9	T10
T11	T12	T13	T14	T15
T16	T17	T18	T19	T20
T21	T22	T23	T24	T25

LEDs

Q1	Q2	Q3	Q4	Q5
Q6	Q7	Q8	Q9	Q10
Q11	Q12	Q13	Q14	Q15
Q16	Q17	Q18	Q19	Q20
Q21	Q22	Q23	Q24	Q25

Other Components

J1	J2	J3	J4	J5
J6	J7	J8	J9	J10
J11	J12	J13	J14	J15
J16	J17	J18	J19	J20
J21	J22	J23	J24	J25

SWITCHES

S1	S2	S3	S4	S5
S6	S7	S8	S9	S10
S11	S12	S13	S14	S15
S16	S17	S18	S19	S20
S21	S22	S23	S24	S25

TEST POINTS

TP1	TP2	TP3	TP4	TP5
TP6	TP7	TP8	TP9	TP10
TP11	TP12	TP13	TP14	TP15
TP16	TP17	TP18	TP19	TP20
TP21	TP22	TP23	TP24	TP25

RESISTORS

R1	R2	R3	R4	R5
R6	R7	R8	R9	R10
R11	R12	R13	R14	R15
R16	R17	R18	R19	R20
R21	R22	R23	R24	R25

CAPACITORS

C1	C2	C3	C4	C5
C6	C7	C8	C9	C10
C11	C12	C13	C14	C15
C16	C17	C18	C19	C20
C21	C22	C23	C24	C25

ICs

U1	U2	U3	U4	U5
U6	U7	U8	U9	U10
U11	U12	U13	U14	U15
U16	U17	U18	U19	U20
U21	U22	U23	U24	U25

DIODES

D1	D2	D3	D4	D5
D6	D7	D8	D9	D10
D11	D12	D13	D14	D15
D16	D17	D18	D19	D20
D21	D22	D23	D24	D25

TRANSISTORS

T1	T2	T3	T4	T5
T6	T7	T8	T9	T10
T11	T12	T13	T14	T15
T16	T17	T18	T19	T20
T21	T22	T23	T24	T25

LEDs

Q1	Q2	Q3	Q4	Q5
Q6	Q7	Q8	Q9	Q10
Q11	Q12	Q13	Q14	Q15
Q16	Q17	Q18	Q19	Q20
Q21	Q22	Q23	Q24	Q25

Other Components

J1	J2	J3	J4	J5
J6	J7	J8	J9	J10
J11	J12	J13	J14	J15
J16	J17	J18	J19	J20
J21	J22	J23	J24	J25

SWITCHES

S1	S2	S3	S4	S5
S6	S7	S8	S9	S10
S11	S12	S13	S14	S15
S16	S17	S18	S19	S20
S21	S22	S23	S24	S25

TEST POINTS

TP1	TP2	TP3	TP4	TP5
TP6	TP7	TP8	TP9	TP10
TP11	TP12	TP13	TP14	TP15
TP16	TP17	TP18	TP19	TP20
TP21	TP22	TP23	TP24	TP25

RESISTORS

R1	R2	R3	R4	R5
R6	R7	R8	R9	R10
R11	R12	R13	R14	R15
R16	R17	R18	R19	R20
R21	R22	R23	R24	R25

CAPACITORS

C1	C2	C3	C4	C5
C6	C7	C8	C9	C10
C11	C12	C13	C14	C15
C16	C17	C18	C19	C20
C21	C22	C23	C24	C25

ICs

U1	U2	U3	U4	U5
U6	U7	U8	U9	U10
U11	U12	U13	U14	U15
U16	U17	U18	U19	U20
U21	U22	U23	U24	U25

DIODES

D1	D2	D3	D4	D5
D6	D7	D8	D9	D10
D11	D12	D13	D14	D15
D16	D17	D18	D19	D20
D21	D22	D23	D24	D25

TRANSISTORS

T1	T2	T3	T4	T5
T6	T7	T8	T9	T10
T11	T12	T13	T14	T15
T16	T17	T18	T19	T20
T21	T22	T23	T24	T25

LEDs

Q1	Q2	Q3	Q4	Q5
Q6	Q7	Q8	Q9	Q10
Q11	Q12	Q13	Q14	Q15
Q16	Q17	Q18	Q19	Q20
Q21	Q22	Q23	Q24	Q25

Other Components

J1	J2	J3	J4	J5
J6	J7	J8	J9	J10
J11	J12	J13	J14	J15
J16	J17	J18	J19	J20
J21	J22	J23	J24	J25

SWITCHES

S1	S2	S3	S4	S5
S6	S7	S8	S9	S10
S11	S12	S13	S14	S15
S16	S17	S18	S19	S20
S21	S22	S23	S24	S25

TEST POINTS

TP1	TP2	TP3	TP4	TP5
TP6	TP7	TP8	TP9	TP10
TP11	TP12	TP13	TP14	TP15
TP16	TP17	TP18	TP19	TP20
TP21	TP22	TP23	TP24	TP25

RESISTORS

R1	R2	R3	R4	R5
R6	R7	R8	R9	R10
R11	R12	R13	R14	R15
R16	R17	R18	R19	R20
R21	R22	R23	R24	R25

CAPACITORS

C1	C2	C3	C4	C5
C6	C7	C8	C9	C10
C11	C12	C13	C14	C15
C16	C17	C18	C19	C20
C21	C22	C23	C24	C25

ICs

U1	U2	U3	U4	U5
U6	U7	U8	U9	U10
U11	U12	U13	U14	U15
U16	U17	U18	U19	U20
U21	U22	U23	U24	U25

DIODES

D1	D2	D3	D4	D5
D6	D7	D8	D9	D10
D11	D12	D13	D14	D15
D16	D17	D18	D19	D20
D21	D22	D23	D24	D25

TRANSISTORS

T1	T2	T3	T4	T5
T6	T7	T8	T9	T10
T11	T12	T13	T14	T15
T16	T17	T18	T19	T20
T21	T22	T23	T24	T25

LEDs

Q1	Q2	Q3	Q4	Q5
Q6	Q7	Q8	Q9	Q10
Q11	Q12	Q13	Q14	Q15
Q16	Q17	Q18	Q19	Q20
Q21	Q22	Q23	Q24	Q25

Other Components

J1	J2	J3	J4	J5
J6	J7	J8	J9	J10
J11	J12	J13	J14	J15
J16	J17	J18	J19	J20
J21	J22	J23	J24	J25

SWITCHES

S1	S2	S3	S4	S5
S6	S7	S8	S9	S10
S11	S12	S13	S14	S15

July 25/06